

Georgia-Pacific



CHLORINE CARTRIDGE



For use with Georgia-Pacific FLOAT
floats for swimming pools.

For use with Georgia-Pacific FLOAT
(Also a replacement for Chem-Lab KEM-2 Chlorine Cartridge)

Active Ingredient: Trichloro-s-Triazinetrione 82%

Inert Ingredients: 18%

(Available Chlorine 73%)

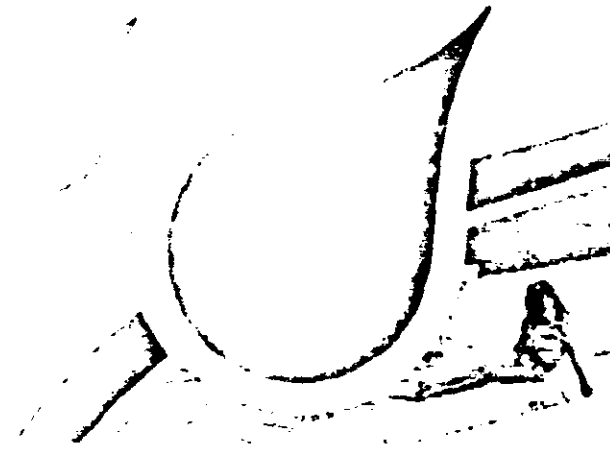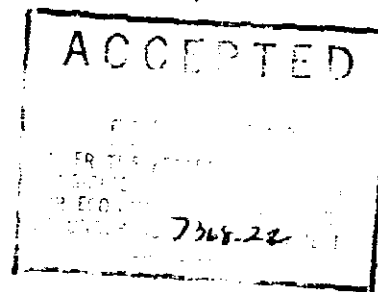

NET WT. 4 LBS.

DANGER: KEEP OUT OF REACH OF CHILDREN

See back panel for precautions.

BEST DOCUMENT.A4

REST DOCUMENT AVAILAE!

GEORGIA PACIFIC CHLORINE CARTRIDGE provides a very simple method of sanitizing your pool by dissolving controlled amounts of chlorine automatically over several weeks time. This makes it much more convenient to use than any liquid or granular forms of chlorine added to the pool several times weekly. The cartridge contains uniform slow-dissolving tablets which contact water only at the bottom of the cartridge. As the bottom tablets dissolve, they are replaced by tablets in the dry reservoir above them, making chlorine addition to the pool constant.

DIRECTIONS FOR USE

1. STABILIZE pool with G-P Conditioner (cyanuric acid)*. Omit if this has been done previously.
 2. CHECK RESIDUAL CHLORINE with a reliable test kit. Remove tape covering holes in side of cartridge. If reading is below 1.0 part per million (PPM), place cartridge at double the feed setting in the table below. Recheck residual chlorine 24 hours later; leave cartridge at this setting until a chlorine residual of 1.0 to 1.5 is established. (Pool should not be used until a residual chlorine of 1.0 PPM minimum is established.)

3. MAINTAIN FEED SETTING by placing cartridge at the setting in the table below. Since chlorine demand is affected by many factors (swimmer load, water temperature, etc.), this setting must be "fine tuned" to your conditions. Check residual chlorine daily and change setting if necessary until 1.0-1.5 PPM chlorine is maintained. From then checks are needed less frequently, but be alert for changes in conditions such as greatly increased swimmer load or much higher temperatures, which may require you to increase setting. The table below shows approximately how long you can expect one cartridge to last. Always keep a replacement on hand.

4. MEASURE pH immediately and at least once each week with a reliable pool test kit. Adjust pH to 7.2-7.8 if necessary by adding Liquid Acid or G-P Dry Acid* to reduce pH, or by adding G-P Soda Ash to increase pH*.

*Follow Directions for Use on labels of these products.

FEED SETTING TABLE

Pool capacity, Gallons	Feed Setting	Approximate number of weeks for one cartridge
5,000	2	8
10,000	3	6
20,000	4	4
25,000	5	3½
30,000	6	3
35,000	7	2½
40,000	8	2

HOW TO CALCULATE POOL CAPACITY

- Rectangular. Average depth x average length x average width x 7.5
- Circular. Diameter x diameter x average depth x 5.9
- Oval with straight sides. Full width x full length x average depth x 6.7
- Irregular. Consult pool builder

1. It is good practice to "superchlorinate" each 2-4 weeks, or at least after each cartridge. To superchlorinate, add ½ gallon Top Chlor Liquid Swimming Pool Chlorine or 10 oz. G-P Dry Chlorine per 10,000 gallons pool capacity. Remove cartridge from pool or place at "0" setting until residual chlorine falls to 1.0-1.5 PPM, then resume regular setting.

2. GEORGIA-PACIFIC CHLORINE CARTRIDGE contains "built-in" Conditioner (cyanuric acid). If it is used regularly, no further additions of G-P Conditioner will be required.

This product is toxic to fish. Treated effluent should not be discharged where it will drain into lakes, streams, ponds, or public water. Do not contaminate water by cleaning of equipment or disposal of wastes. Apply this product only as specified on this label.

DANGER: CORROSIVE. Causes eye damage. May cause burns on moist or broken skin. Do not get in eyes, on skin, or on clothing. May be harmful or fatal if swallowed.


Strong oxidizing agent. Contact with heat, moisture, foreign material, other chemicals, or contamination from any source may result in fire or explosive decomposition. Will burn with evolution of hazardous and irritating chlorine-containing gases. Avoid contamination with combustible materials or moisture. Keep away from heat and open flames. Store product in tightly-closed container in a cool, dry place when not in use. In case of fire, isolate container in well-ventilated area and flood with water. Do not refill this container. Rinse empty container thoroughly with water and discard it.

FIRST AID: In case of contact, immediately flush eyes or skin with plenty of water for at least 15 minutes. For eyes call a physician. Remove and wash contaminated clothing before reuse.

If swallowed, drink promptly a large quantity of milk, egg whites, gelatin solution, or if these are not available, drink large quantities of water. Avoid alcohol. Call a physician immediately.

EPA Reg. No. 7368-22-AA
 Another quality product from

Georgia-Pacific 
 Los Angeles, Calif. 90040

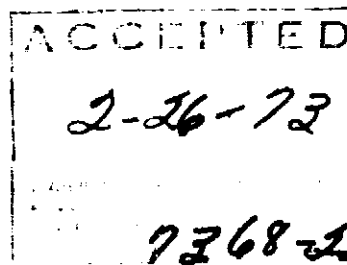

LABEL COPY

CHLORINE CARTRIDGE EPA REG. NO. 7368-22.

Label copy to be the same as that accepted February 26, 1973 with following exceptions:


1. Active ingredient: Trichloro-S-Triazinetrione 100% (Available Chlorine 89%).
2. Net wt. 5 lbs. (Formerly 4 lbs.)
3. We will make the revision requested in the Notice of Registration, issued 3/1/73.
4. Feed Setting Table

<u>Pool Capacity Gallons</u>	<u>Feed Setting</u>	<u>Approximate number of Weeks for one Cartridge</u>
5,000	2	12
10,000	3	9
20,000	4	6
25,000	5	5
30,000	6	4 1/2
35,000	7	3 1/2
40,000	8	3

Note to EPA: "Approximate Number of Weeks" column is increased by 1/2 because total Chlorine content of Cartridge is increased as follows:

Formerly 73% available Chlorine x 4 lbs. = 2.92 lbs.
 New 89% available Chlorine x 5 lbs. = 4.45 lbs.

$$\frac{4.45}{2.92} = 1.52$$

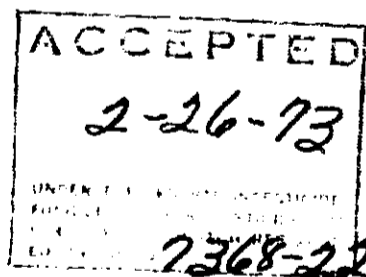

D.W.C.
 D. W. C.
 12/6/73

GEORGIA-PACIFIC CHLORINE CARTRIDGE provides a very simple method of sanitizing your pool by dissolving controlled amounts of chlorine automatically over several weeks time. This makes it much more convenient to use than any liquid or granular forms of chlorine added to the pool several times weekly. The cartridge contains uniform slow-dissolving tablets which contact water only at the bottom of the cartridge. As the bottom tablets dissolve, they are replaced by tablets in the dry reservoir above them, making chlorine addition to the pool constant.

DIRECTIONS FOR USE

1. **STABILIZE** pool with G-P Conditioner (cyanuric acid)*. Omit if this has been done previously.
2. **CHECK RESIDUAL CHLORINE** with a reliable test kit. Remove tape covering holes in side of cartridge. If reading is below 1.0 part per million (PPM), place cartridge at **double** the feed setting in the table below. Recheck residual chlorine 24 hours later; leave cartridge at this setting until a chlorine residual of 1.0 to 1.5 is established. (Pool should not be used until a residual chlorine of 1.0 PPM minimum is established.)
3. **MAINTAIN RESIDUAL CHLORINE** by placing cartridge at the setting in the table below. Since chlorine demand is affected by many factors (swimmer load, water temperature, etc.), this setting must be "fine tuned" to your conditions. Check residual chlorine daily and change setting if necessary until 1.0—1.5 PPM chlorine is maintained. From then checks are needed less frequently, but be alert for changes in conditions such as greatly increased swimmer load or much higher temperatures, which may require you to increase setting. The table below shows **approximately** how long you can expect one cartridge to last. Always keep a replacement on hand.
4. **MEASURE pH** immediately and at least once each week with a reliable pool test kit. Adjust pH to 7.2—7.8 if necessary by adding Liquid Acid or G-P Dry Acid* to reduce pH, or by adding G-P Soda Ash to increase pH*.

*Follow Directions for Use on labels of these products.

FEED SETTING TABLE

Pool capacity, Gallons	Feed Setting	Approximate number of weeks for one cartridge
5,000	2	8
10,000	3	6
20,000	4	4
25,000	5	3½
30,000	6	3
35,000	7	2½
40,000	8	2

ACCEPTED
 2-26
 UNDER THE
 FINGERPRINT

LABEL COPY

CHLORINE CARTRIDGE EPA REG. NO. 7368-22.

Label copy to be the same as that accepted February 26, 1973 with following exceptions:


1. Active ingredient: Trichloro-S-Triazinetrione 100% (Available Chlorine 89%).
2. Net wt. 5 lbs. (Formerly 4 lbs.)
3. We will make the revision requested in the Notice of Registration, issued 3/1/73.
4. Feed Setting Table

<u>Pool Capacity Gallons</u>	<u>Feed Setting</u>	<u>Approximate number of Weeks for one Cartridge</u>
5,000	2	12
10,000	3	9
20,000	4	6
25,000	5	5
30,000	6	4 1/2
35,000	7	3 1/2
40,000	8	3

Note to EPA: "Approximate Number of Weeks" column is increased by 1/2 because total Chlorine content of Cartridge is increased as follows:

Formerly 73% available Chlorine x 4 lbs. = 2.92 lbs.
 New 89% available Chlorine x 5 lbs. = 4.45 lbs.

$$\frac{4.45}{2.92} = 1.52$$

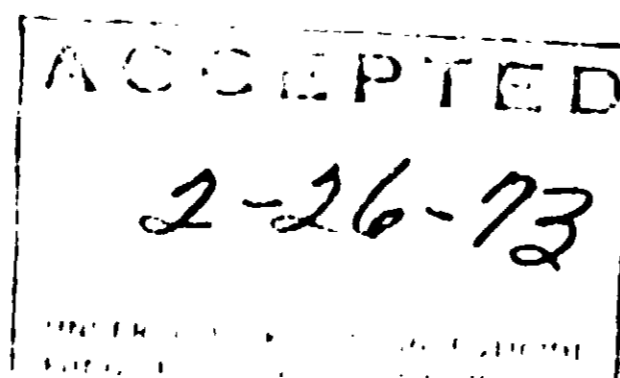

DIV-
 D. W. C.
 12/6/73

A