



Distributed exclusively by  
W. T. Grant Co., New York, New York 10036

509-008

**TASK FORCE GRANULAR CHLORINE FOR EFFECTIVE CONTROL OF BACTERIA AND ALGAE  
POOL START-UP (PRE-CONDITIONING) INSTRUCTIONS**

The Task Force pool chemical program makes pool sanitizing easy, economical and effective. When first filling your new pool or refilling with fresh water at anytime: 1. Test water for pH level; 2. Adjust pH to a range of 7.2 to 7.6 with Task Force Dry Acid or Soda Ash as required; 3. Condition pool water with Task Force Water Conditioner; 4. Shock treat pool water by adding Task Force Granular Chlorine at the rate of 3 oz. per 2500 gallons of water. Allow the chlorine reading to drop 2 to 3 ppm (1 to 2 for unstabilized water) on your Task Force Test Kit before entering pool.

**DAILY MAINTENANCE INSTRUCTIONS**

For proper protection, the chlorine residual of your pool water should be maintained in a range between 2.0 to 3.0 ppm as indicated by your Task Force Test Kit. The table below shows recommended daily dosages to maintain this range for pools used under average load and weather conditions. Slight increases in chlorine dosage may be required to meet the extra demands resulting from heavy bathing loads, accumulations of dust and dirt caused by storms, or continued high temperatures.

**RECOMMENDED DAILY DOSAGES FOR PROPERLY  
PRE-CONDITIONED POOLS**

Amount to add daily by pool size in gallons, use graduated 1 oz. measuring cup provided in container.

Test Kit Reading	2500 gals.	5000 gals.	7500 gals.	10,000 gals.	12,500 gals.	15,000 gals.	17,500 gals.	20,000 gals.
0 to 1.0	1/4 cup	1 cup	1 1/2 cups	2 cups	2 1/2 cups	3 cups	3 1/2 cups	4 cups
1.0 to 2.0	1/4 cup	1/2 cup	3/4 cup	1 cup	1 1/4 cups	1 1/2 cups	1 3/4 cups	2 cups

These dosages are for average conditions. Test your pool water for chlorine level daily and adjust as required.



For maximum protection, shock treat your pool every two weeks. Follow step 4 above.

**"DANGER" KEEP OUT OF REACH OF CHILDREN**

**CORROSIVE:** Causes eye damage. May cause burns on broken skin. Do not get in eyes, on skin or on clothing. May be irritating or harmful if inhaled. Avoid breathing dust. May be harmful or fatal if swallowed.

**STRONG OXIDIZING MATERIAL:** Contact with heat, moisture, foreign material or contamination from any source may result in fire. Will burn with the evolution of hazardous and irritating chlorine-containing gases. Avoid contamination with combustible materials. Keep away from open flames and heat. Use only dry, clean measures. Mix only with water. Keep closed when not in use. Store in cool, dry place. Do not reuse container — rinse thoroughly clean with water before discarding.

**FIRST AID.** Internal—feed cooked cereal or bread soaked in milk, followed by olive oil or cooking oil. "CALL A PHYSICIAN IMMEDIATELY." External—in case of contact, immediately flush eyes or skin with cold water for at least 15 minutes. For eyes, call a physician.

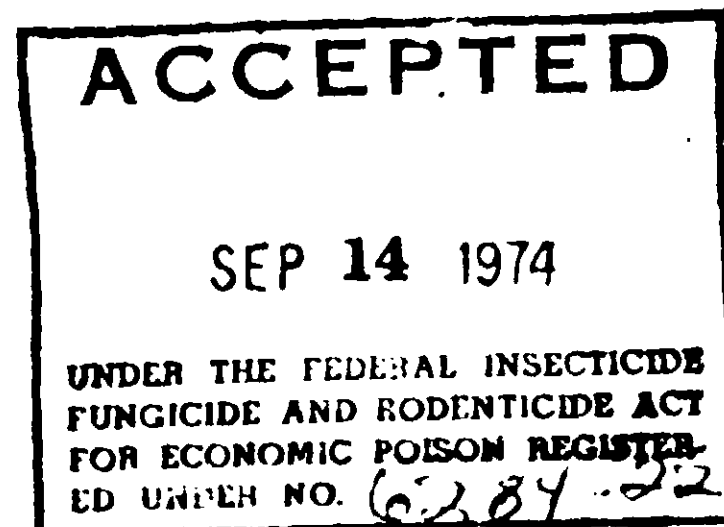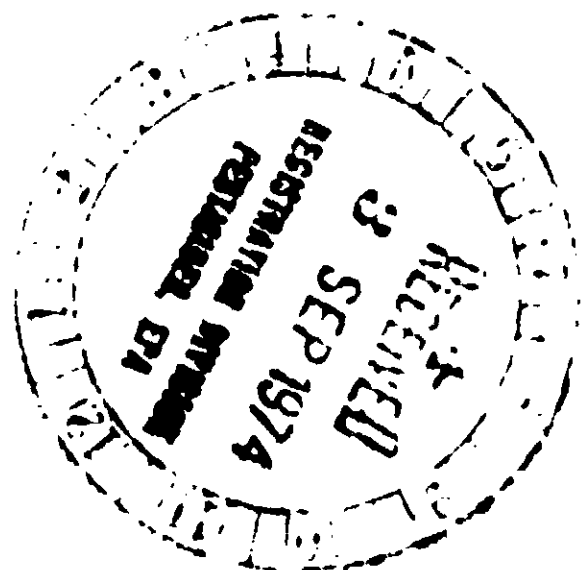

Cameraman's Note

Poor Copy



Distributed exclusively by  
W. T. Grant Co., New York, New York 10036

508-008

**TASK FORCE GRANULAR CHLORINE FOR EFFECTIVE CONTROL OF BACTERIA AND ALGAE  
POOL START-UP (PRE-CONDITIONING) INSTRUCTIONS**

The Task Force pool chemical program makes pool sanitizing easy, economical and effective. When first filling your new pool or refilling with fresh water at anytime: 1. Test water for pH level; 2. Adjust pH to a range of 7.2 to 7.6 with Task Force Dry Acid or Soda Ash as required; 3. Condition pool water with Task Force Water Conditioner; 4. Shock treat pool water by adding Task Force Granular Chlorine at the rate of 3 oz. per 2500 gallons of water. Allow the chlorine reading to drop 2 to 3 ppm (1 to 2 for unstabilized water) on your Task Force Test Kit before entering pool.

**DAILY MAINTENANCE INSTRUCTIONS**

For proper protection, the chlorine residual of your pool water should be maintained in a range between 2.0 to 3.0 ppm as indicated by your Task Force Test Kit. The table below shows recommended daily dosages to maintain this range for pools used under average load and weather conditions. Slight increases in chlorine dosage may be required to meet the extra demands resulting from heavy bathing loads, accumulations of dust and dirt caused by storms, or continued high temperatures.

**RECOMMENDED DAILY DOSAGES FOR PROPERLY  
PRE-CONDITIONED POOLS**

Amount to add daily by pool size in gallons, use graduated 1 oz. measuring cup provided in container.

Test Kit Reading	5000 gals.	6000 gals.	7500 gals.	10,000 gals.	12,500 gals.	15,000 gals.	17,500 gals.	20,000 gals.
0 to 1.0	1/2 cup	1 cup	1 1/2 cups	2 cups	2 1/2 cups	3 cups	3 1/2 cups	4 cups
1.0 to 2.0	1/4 cup	1/2 cup	3/4 cup	1 cup	1 1/4 cups	1 1/2 cups	1 3/4 cups	2 cups

These dosages are for average conditions. Test your pool water for chlorine level daily and adjust as required.

For maximum protection, shock treat your pool every two weeks. Follow step 4 above.

**"DANGER" KEEP OUT OF REACH OF CHILDREN**

**CORROSIVE:** Causes eye damage. May cause burns on broken skin. Do not get in eyes, on skin or on clothing. May be irritating or harmful if inhaled. Avoid breathing dust. May be harmful or fatal if swallowed.

**STRONG OXIDIZING MATERIAL:** Contact with heat, moisture, foreign material or contamination from any source may result in fire. Will burn with the evolution of hazardous and irritating chlorine-containing gases. Avoid contamination with combustible materials. Keep away from open flames and heat. Use only dry clean measures. Mix only with water. Keep closed when not in use. Store in cool, dry place. Do not reuse container — rinse thoroughly clean with water before discarding.

**FIRST AID:** Internal — feed cooked cereal or bread soaked in milk, followed by olive oil or cooking oil. "CALL A PHYSICIAN IMMEDIATELY."  
Eyes — in case of contact, immediately flush eyes or skin with cold water for at least 15 minutes. For eyes, call a physician.



**ACCEPTED**

SEP 14 1974

UNDER THE FEDERAL INSECTICIDE  
FUNGICIDE AND RODENTICIDE ACT  
FOR ECONOMIC POISON REGISTERED  
ED UNDER NO. 62-287-22