

SEABOARD

sea/chlor

DRY CHLORINE SANITIZER FOR ALL SWIMMING POOLS

- Easy to Use • Just Pour into Pool
- Clears Water Instantly • Completely Soluble
- Highly Effective Bactericide and Disinfectant


Contains 35 % available chlorine.

Active Ingredient, lithium hypochlorite 29%
Inert Ingredients 71%


WARNING: Keep out of children's reach
SEE SIDE PANEL FOR ADDITIONAL PRECAUTIONS.

EPA REG. NO. 7152-15

Net.Wt. 4 1/2 Lbs.



SEABOARD
INDUSTRIES
HAWTHORNE, NEW JERSEY

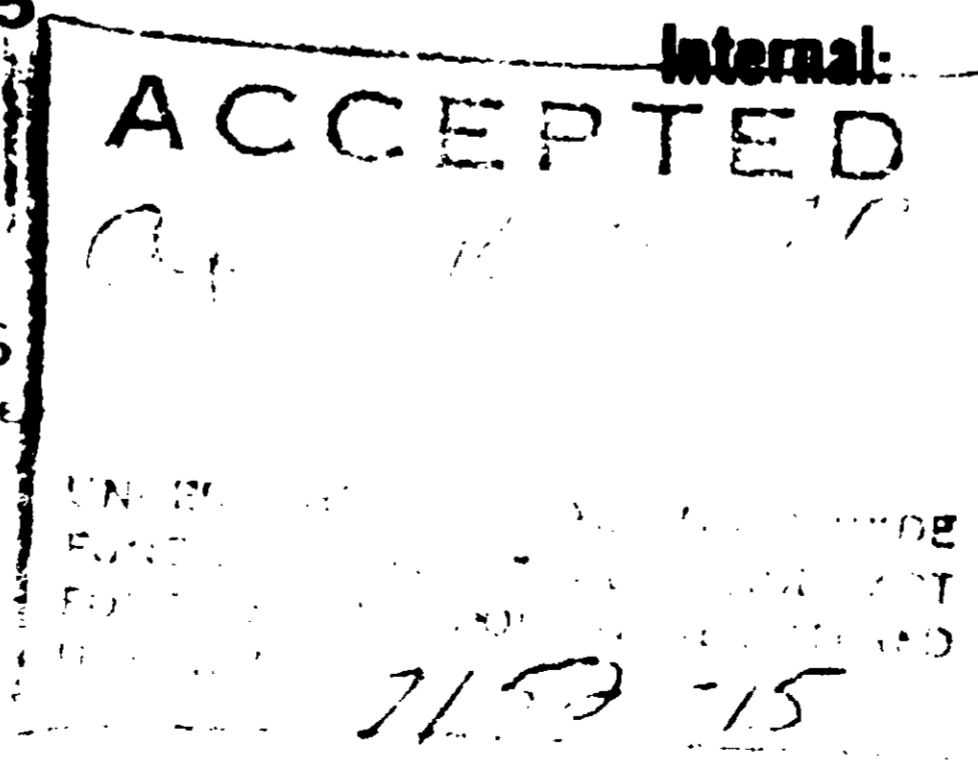

HOW TO STORE AND HANDLE CHLORINE SANITIZER

- Store in a cool, dry place. Do not transfer into unlabeled containers. Close containers tightly after each use.
- Protect from moisture and heat.
- Add material only to water.
- May cause fire or explosion if mixed with other chemicals.
- Use only glass, plastic or enamel ware cups and spoons in measuring product. Make sure they are clean and dry. Wash hands thoroughly with water after use. If spilled, hose down thoroughly. Never dispose of material by throwing into refuse bins.
- Rinse empty container thoroughly with water and discard it.

WARNING: May be fatal or harmful if swallowed. Strong oxidant. May produce chemical burns. Do not handle with wet hands. Fire may result from contact with acids, organic or combustible matter. Do not get on skin or in eyes.

FIRST AID:

External: In case of skin and eye contact, flush with plenty of water. If skin irritation persists, get medical attention. For eyes, get prompt medical attention.

Internal: If swallowed, drink milk, raw egg white, milk or rice gruel. Follow with emetic (tablespoon or mustard in a glass of warm water). CALL A PHYSICIAN IMMEDIATELY.

INSTRUCTIONS FOR USE:

1. Adjust the pool water pH to 7.2 to 7.6 as necessary with "PLUS" or "MINUS".
2. Superchlorinate to satisfy chlorine demand and to establish a chlorine residual of 1.0 to 1.5 PPM. To accomplish this, add 2.0 oz. of "JOLT-IT" Shock Treatment per every 1000 gallons of pool water.
3. Test pool water after 4 hours with a chlorine test kit. If there is no chlorine residual, recheck pH with test kit and readjust as in step No. 1. Then repeat above chlorine dosage until a reading of 1.0 to 1.5 PPM is determined by test kit.
4. Water should be superchlorinated every two weeks when temperature of water is below 80°F., and weekly when tempera-

ture is above 80°F. This is best done in the evening when the pool will not be in use for a minimum of 12 hours. In the morning, check available chlorine with a chlorine test kit, and maintain a chlorine residual of 1.0 to 1.5 PPM.

5. After a chlorine residual has been established, condition the pool by adding 4 oz. of cyanuric acid to every 1000 gallons of water.
6. If chlorine residual is above 2.0 PPM, do not allow swimming until residual is decreased below 2.0 PPM.
7. Add your regular swimming pool sanitizer according to package directions to maintain a minimum chlorine residual of 1.0 to 1.5 PPM at all times.

CAUTION: This product is toxic to fish. Treated pool effluent water should not be discharged where it will drain into lakes, streams, ponds or public water.

Do not contaminate water by cleaning of equipment or disposal of wastes.

SEABO JOLT SHOCK TR

ACTIVE INGREDIENT:
Sodium Dichloro-S-Triazinetrione

Available Chlorine

EPA REG. No.

DANGER KEEP OUT OF
SEE SIDE PANEL FOR FIRST
PRECAUTIONS
NET WT. 4

REPACKED BY:



SEABO
INDUS
HAWTHORNE