

1-15/91-14/1

10/1

### DIRECTIONS FOR USE:

For complete sterilization or disinfection of medical instruments and equipment, thoroughly clean, rinse and rough-dry objects before immersing in full strength solution. Cleanse and rinse the lumens of any hollow instruments before filling with solution. Avoid entrapment of air bubbles.

Disinfection: Immerse instruments or equipment completely for a minimum of 10 minutes at 20°C to destroy vegetative organisms including *Pseudomonas aeruginosa*, *Staphylococcus aureus*, *Salmonella choleraesuis*, and pathogenic fungi as represented by *Trichophyton mentagrophytes*. For 100% kill of *Mycobacterium tuberculosis*, immerse instruments or equipment completely for a minimum of 20 minutes at 20°C, or 10 minutes at 25°C. **VIRUSES:**

The following viruses are completely inactivated in 3 minutes at 20°C: Cytomegalovirus; Respiratory Syncytial Virus; Rhinovirus; Rotavirus SA-11; Herpes simplex virus 1 & 2; Adenovirus 2; Coxsackievirus B5a; Echovirus 8; Poliovirus 1 & 2; Vaccinia virus; Influenza A<sub>2</sub> HK. After immersion, remove instruments or equipment from METRICIDE Solution and rinse thoroughly. All times and temperatures are based on EPA-approved testing on inanimate surfaces.

Sterilization: Immerse instruments or equipment completely for a minimum of 8 hours at 20°C to destroy resistant pathogenic spores as represented by *Clostridium sporogenes* and *Bacillus subtilis*. Remove instruments or equipment from METRICIDE Solution using sterile technique and rinse thoroughly with sterile water.

### DIRECTIONS FOR ACTIVATION:


Add contents of attached vial to this container of METRICIDE Solution. Shake. Solution is ready to use. When activated, solution changes color to green. This solution may be used and reused for up to 14 days after activation. Do not use activated stock solution beyond 14 days.

General Classification - For use in Hospitals, Dental Offices, Nursing Homes and Health Care Institutions. For repeated use in manual (bucket and tray) systems. This product is not formulated as a "holding" solution. It is a violation of Federal Law to use this product in a manner inconsistent with its labeling.

Product No.	MX-1405
Active ingredient	Glutaraldehyde 2.0%
Inert ingredients	98.0%
Total	100.0%

MIXING DATE  
EXPIRATION DATE

E.P.A. Reg. No. 46781-1  
E.P.A. Est. No. 46781-CO-1

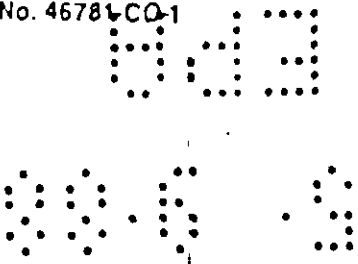

## REUSABLE Sterilizing and Disinfecting Solution

Rapid-acting • Non-staining • Non-rusting


# METRICIDE

Activated Dialdehyde Solution

## Sporicidal Fungicidal Bactericidal Virucidal Tuberculocidal Pseudomonacidal

**DANGER: Keep out of reach of children.**  
See right side panel for precautions.  
Note: Contents of attached vial must be added to fluid before this product is effective.  
See directions for activating

\*See directions for use

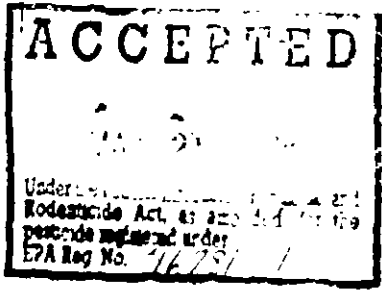

### PRECAUTIONARY STATEMENTS:

**DANGER: Hazard to Humans**  
Follow All Label Directions

**Eyes** - Contact with eyes causes damage. In case of contact, flush with water immediately and get medical attention.  
**Skin** - Avoid skin contact as possibility of sensitization exists. May cause skin irritation. For skin contact flush thoroughly with water.  
**Ingestion** - Avoid contamination of food. Harmful if swallowed.  
**Inhalation** - Use in ventilated area.


### STORAGE AND DISPOSAL:

Keep in a cool place. Do not reuse empty container. Wrap container and put in trash.

- \* Especially recommended for sterilization or disinfection of:
  - Lensed instruments
  - Anesthesia equipment
  - Respiratory therapy equipment
  - Rubber objects
  - Plastic objects
  - Sharp instruments
  - Thermometers
  - Flexible fiberoptic endoscopes

Contents One Qt. (32 fluid oz.)  
Made in U.S.A.  
Control Number on Bottom

Manufactured by



DK BLUE 270

**BEST AVAILABLE COPY**