



STATE OF IDAHO
DEPARTMENT OF
ENVIRONMENTAL QUALITY

1410 North Hilton • Boise, Idaho 83706 • (208) 373-0502
www.deq.idaho.gov

C.L. "Butch" Otter, Governor
John H. Tippetts, Director

August 12, 2015

Mr. Keith Rose
Environmental Scientist
U.S. EPA, Region 10
1200 Sixth Ave.
Seattle, WA 98101

RE: Final Annual Monitoring Network Review - 2015

Dear Mr. Rose:

Idaho Department of Environmental Quality (DEQ) is submitting to EPA Region 10 the *2015 Annual Ambient Air Quality Monitoring Network Plan (Plan)*, per the requirements of 40 CFR §58.10. A draft of the plan was sent to you on July 1, 2015. This submittal satisfies the conditions of the CY15 base grant Workplan. The enclosed *Plan* addresses all monitoring requirements for NCore stations as well as non-source oriented lead (Pb) monitoring, as required in subsections 58.10.a.3 and 58.10.a.4.

This *Plan* was made available for a thirty (30) day public comment period as required in 40 CFR §58.10. The 30-day comment period ended July 31, 2015. No comments were received.

Please let me know if you have any questions or requests. I can be reached at (208) 373-0432.

Sincerely,


A handwritten signature in black ink, appearing to read "Steve Miller".

Steve Miller
Air Quality Monitoring Coordinator
Idaho Department of Environmental Quality

Enclosure(s) 1

c: Chris Hall, EPA, Air QA Coordinator
Tiffany Floyd, AQ Division Administrator
Bruce Louks, AQ Manager, MMEI
Mary Grandjean, AQ Grants Administrator

Idaho Department of Environmental Quality Annual Ambient Air Quality Monitoring Network Plan

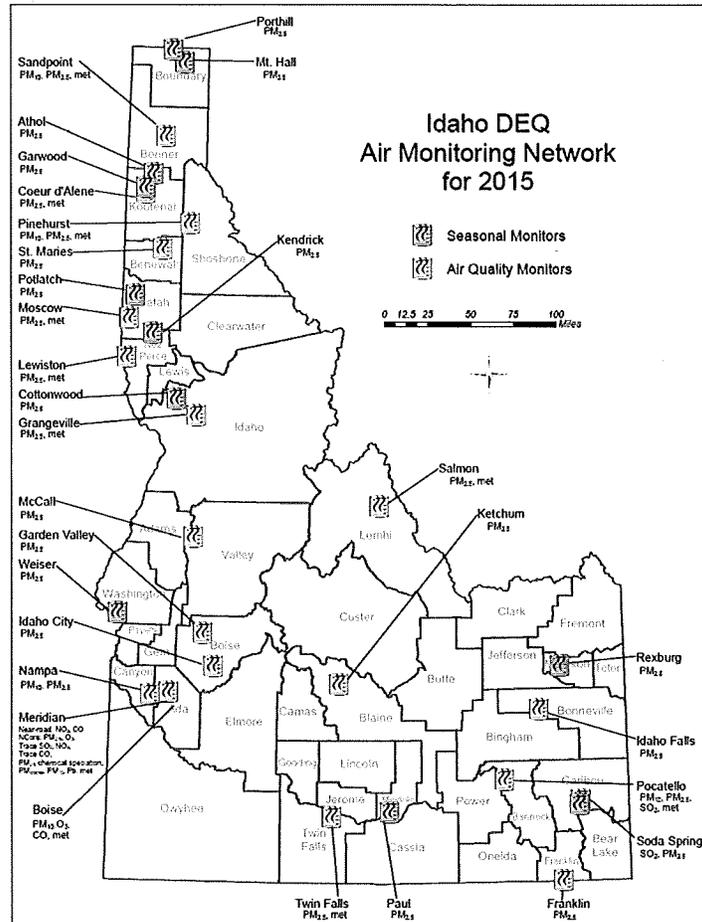

**State of Idaho
Department of Environmental Quality**

July 2015



*Printed on recycled paper, DEQ July 2015,
PID MPOP, CA code 81631. Costs associated with
this publication are available from the State of Idaho
Department of Environmental Quality in accordance
with Section 60-202, Idaho Code.*

Idaho Department of Environmental Quality Annual Ambient Air Quality Monitoring Network Plan

July 2015



**Prepared by
Idaho Department of Environmental Quality
Air Quality Division
1410 North Hilton
Boise, Idaho 83706**

This page intentionally left blank for correct double-sided printing.

Contents

Executive Summary	v
1 Introduction.....	1
2 Air Quality Surveillance Systems and Monitoring Objectives.....	2
3 Idaho DEQ’s Ambient Air Monitoring Network.....	4
3.1 Monitoring Sites	5
3.2 DEQ Monitoring Network—Monitoring Purpose, Scale of Representativeness, and Area Represented	8
3.3 Monitoring Methods, Monitor Designation, and Sampling Frequency	12
4 DEQ Network Modifications Subsequent to the EPA-Approved 2014 Ambient Monitoring Network Plan	19
5 Proposed Network Modifications	20
5.1 PM ₁₀ Monitoring Network.....	20
5.2 PM _{2.5} Core NAAQS Compliance Monitoring Network.....	21
5.3 PM _{2.5} Continuous Monitoring Network	21
5.4 Ozone Monitoring Network	22
5.5 Carbon Monoxide (CO) Monitoring Network	23
5.6 Sulfur Dioxide (SO ₂) Monitoring Network.....	23
5.7 Nitrogen Dioxide (NO ₂) Monitoring Network	24
5.8 Lead (Pb) Monitoring Network	24
5.9 PM _{10-2.5} (PM _{coarse}).....	24
5.10 Summary of Proposed Network Modifications for DEQ’s 2015 Air Monitoring Network Plan	25
6 Future Ambient Air Monitoring Requirements and Associated Costs.....	25

Appendices

- Appendix A. DEQ Ambient Monitoring Network Design Values
- Appendix B. Craters of the Moon and Hells Canyon Monitoring Stations (Improve Network)
- Appendix C. EPA-DEQ Correspondence
- Appendix D. 40 CFR Part 58—Appendix D and E Checklists

List of Tables

Table 1. DEQ monitoring stations, locations, and AQS identification codes.....	6
Table 2. CRB station locations.	7
Table 3. Relationships between site types and scales of representativeness.	9
Table 4. Monitoring objectives, areas represented, and scales of representation.	10
Table 5. Air monitoring method codes.	13
Table 6. Site summary including pollutants monitored, monitor designation, monitoring frequency, and method codes.	16
Table 7. DEQ meteorological monitoring stations and parameters.	19

List of Figures

Figure 1. Idaho air quality monitoring network, 2015.....	5
Figure 2. Minimum monitoring frequency based on ratio of local concentration to standard. (Note: DV = design value.)	15

Executive Summary

The main objective of the Idaho Department of Environmental Quality's (DEQ's) 2015 annual ambient air monitoring network plan is to determine whether the state's ambient air monitoring network is achieving its monitoring objectives and to identify any needed modifications.

DEQ is proposing the following network modifications:

- Based on the most recent 2012–2014 24-hour design value, change the St. Maries Federal Reference Method (FRM) monitor's run schedule from 1/6 days to 1/1 days, effective no later than January 1, 2016.
- Based on the most recent 2012–2014 24-hour design value, change the Nampa Fire Station FRM monitor's run schedule from 1/6 days to 1/3 days, effective no later than January 1, 2016.
- Pending final US Environmental Protection Agency (EPA) ruling as part of 40 CFR Part 58 monitoring requirement revisions, discontinue lead monitoring at DEQ's NCore site, upon EPA approval.
- At a minimum, relocate the Eastman carbon monoxide monitor inlet a minimum of 2 meters from the nearest traffic lane. If not possible, research moving site to a new location.
- Relocate the Franklin 1405-F tapered element oscillating microbalance (TEOM) monitor to the Pocatello Garrett & Gould site, where its very sharp cut cyclone (VSCC) will be replaced by a sharp cut cyclone (SCC). This change will make it a special purpose monitor (SPM) for Air Quality Index (AQI) reporting.

Since submitting the 2014 plan, DEQ has made the following subsequent modifications to the network. Some items required EPA approval, while other less significant items did not.

- The St. Maries beta attenuation monitor (BAM) 1020 (start date of January 1, 2014) is no longer being tested for federal equivalent method (FEM) comparability. DEQ decided to designate it an SPM for AQI and smoke management and is continuing to use the FRM at St. Maries as the National Ambient Air Quality Standard (NAAQS) monitor. The BAM was converted to an SPM by switching the impactor from a VSCC to an SCC.
- The Pinehurst and Salmon FRM monitors have been designated the primary NAAQS monitors as of January 1, 2015.
- The St. Luke's Speciation Air Sampling System monitor PM_{2.5} (fine particulate) mass measurement has been discontinued per EPA final ruling.

This page intentionally left blank for correct double-sided printing.

1 Introduction

This document, in accordance with the federal requirements described below, is the Idaho Department of Environmental Quality's (DEQ's) 2015 annual ambient air quality monitoring network plan. The primary goal of the annual network plan is to determine whether the state monitoring network is achieving its monitoring objectives and to identify any needed modifications. The appendices provide additional information on network design values (Appendix A), the IMPROVE monitoring network (Appendix B), supplemental correspondence (Appendix C), and federal requirement checklists (Appendix D).

Idaho's monitoring network has four principal objectives: (1) assess compliance with National Ambient Air Quality Standards (NAAQS); (2) support smoke management programs, including agricultural and prescribed burning practices; (3) identify emergency episodes caused by wind-blown dust or wildfire; and (4) support the evaluation of state implementation and maintenance plans (SIPs). In addition, DEQ operates a network of continuous fine particulate (PM_{2.5}) monitors and surface meteorology stations to support air quality forecasting, the Air Quality Index (AQI) program, and modeling projects. DEQ also leverages the IMPROVE monitoring network to fulfill requirements for the PM_{2.5} transport (Hells Canyon) and PM_{2.5} background (Craters of the Moon National Monument) monitoring sites (Appendix B).

Beginning July 1, 2007, state agencies were required to adopt and submit to the US Environmental Protection Agency (EPA) regional administrator an annual monitoring network plan (40 CFR §58.10). The plan shall provide for the establishment and maintenance of an air quality surveillance system that consists of a network made up of the following types of monitoring stations:

- State and local air monitoring stations (SLAMS), including monitors that use the following methods:
 - Federal reference method (FRM)
 - Federal equivalent method (FEM)
 - Approved regional method (ARM)
- NCore stations (included in the national network of multipollutant monitoring stations)
- PM_{2.5} (particulate matter with diameter ≤ 2.5 microns [μ]) chemical speciation stations (STN)
- Special purpose monitoring (SPM) stations

This plan also lists seasonal fine particulate (PM_{2.5}) monitors used for smoke and agricultural burning management.

The plan shall include a statement of purposes for each monitor and evidence that siting and operation of each monitor meets the requirements of Appendices A, C, D, and E of 40 CFR Part 58 where applicable (Appendix D).

This plan was made available for public inspection for 30 days prior to submission to EPA. Any annual monitoring network plan that proposes SLAMS network modifications—including new monitoring sites—is subject to approval by the EPA regional administrator, who shall provide opportunity for public comment and shall approve or disapprove the plan and schedule within

120 days. If the state or local agency has already provided a public comment opportunity on its plan, has made no changes subsequent to that comment opportunity, and has submitted the received comments together with the plan, the regional administrator is not required to provide a separate opportunity for comment.

This 2015 plan includes all required stations to be operational by January 1, 2016. Specific locations for the required monitors are included in this plan.

The annual monitoring network plan contains the following required information for existing and proposed sites where appropriate:

- The AQS (air quality system, EPA's database) site identification number
- The location, including street address and geographical coordinates
- The sampling and analysis method(s) for each measured parameter
- The operating schedules for each monitor
- Any proposals to remove or move a monitoring station within a period of 18 months following plan submittal
- The monitoring objective and spatial scale of representativeness for each monitor as defined in Appendix D to 40 CFR Part 58
- The identification of any sites that are suitable or unsuitable for comparison against the annual PM_{2.5} NAAQS as described in 40 CFR §58.30
- The metropolitan statistical area (MSA), core-based statistical area (CBSA), combined statistical area (CSA), or other area represented by the monitor
- The designation of any lead monitors as either source-oriented or non-source-oriented (i.e., NCore) according to Appendix D to 40 CFR Part 58
- Any source-oriented monitors for which a waiver has been requested or granted by the EPA regional administrator as allowed for under paragraph 4.5(a)(ii) of Appendix D to 40 CFR Part 58
- Any source-oriented or non-source-oriented site for which a waiver has been requested or granted by the EPA regional administrator for the use of lead-PM₁₀ (particulate matter with diameter $\leq 10 \mu$) monitoring in lieu of lead-total suspended particulate (TSP) monitoring as allowed for under paragraph 2.10 of Appendix C to 40 CFR Part 58

The annual monitoring network plan documents how states and local agencies provide for the review of changes to a PM_{2.5} monitoring network that impact the location of a violating PM_{2.5} monitor. The affected state or local agency must document the process for obtaining public comment and include any comments received through the public notification process within their submitted plan.

2 Air Quality Surveillance Systems and Monitoring Objectives

Ambient air monitoring objectives have shifted over time, a situation that requires air quality agencies to re-evaluate and reconfigure monitoring networks. A variety of factors contribute to these shifting monitoring objectives:

- Air quality has changed since adoption of the federal Clean Air Act and NAAQS. For example, the problems of high ambient concentrations of lead and carbon monoxide have largely been solved.
- Populations and behaviors have changed. For example, the US population has (on average) grown, aged, and shifted toward urban and suburban areas over the past four decades. In addition, rates of vehicle ownership and annual miles driven have increased.
- New air quality objectives have been established, including rules to reduce air toxics, fine particulate matter (PM_{2.5}), and regional haze.
- The understanding of air quality issues and the capability to monitor air quality have both improved. Together, the enhanced understanding and capabilities can be used to design more effective air monitoring networks.

Ambient air monitoring networks must be designed to meet three basic monitoring objectives. Each objective is equally important and must be considered individually.

- **Provide air pollution data to the general public in a timely manner.** Data can be presented to the public in a number of ways, including air quality maps, newspaper articles or advertisements, Internet sites, and as part of weather forecasts and public advisories.
- **Provide support for determining compliance with ambient air quality standards and developing emissions control strategies.** Data from qualified monitors for NAAQS pollutants are used for comparing an area's air pollution levels against the NAAQS. Data from monitors of various types can be used in developing attainment and maintenance plans. SLAMS, and especially NCore station data, are used to evaluate the regional air quality models used in developing emission strategies and to track effectiveness of air pollution abatement control measures. In monitoring locations near major air pollution sources, source-oriented monitoring data can provide insight into how well industrial sources are controlling their pollutant emissions.
- **Provide support for air pollution research studies.** Air pollution data from the NCore multipollutant monitoring network can be used to supplement data collected by researchers working on health effects assessments and atmospheric processes or for monitoring methods development work.

To support the air quality management work indicated in the three basic air monitoring objectives, a network must be designed with a variety of monitoring site types. Monitoring sites must be capable of informing airshed managers about many things including the peak air pollution levels, typical levels in populated areas, air pollution transported into and outside of a city or region, and air pollution levels near specific emissions sources. These types of sites are summarized in the following list of six general site types:

- Maximum concentrations of air pollutants expected to occur in the area covered by the network
- Typical pollutant concentrations in areas of high population density
- Impact of significant sources or source categories on air quality
- General background concentration levels of air pollutants
- Extent of regional pollutant transport among populated areas and compliance with secondary air quality standards
- Air pollution impacts on visibility, vegetation damage, or other welfare-based impacts

The adequacy of an ambient air monitoring network may be determined by using a variety of tools, including the following:

- Federal monitoring requirements and network minimums
- Analyses of historical monitoring data
- Maps of pollutant emissions densities
- Dispersion modeling
- Special studies/saturation sampling
- SIP requirements
- Revised monitoring strategies (e.g., new regulations, reengineering of the air monitoring network)
- Network maps and network descriptions with site objectives defined
- Best professional judgment

The appropriate location of a monitor can only be determined on the basis of stated objectives. The following tools can help determine whether monitor locations are meeting their stated objectives:

- Maps, graphical overlays, and information based on geographic information systems (GIS), which are extremely helpful for visualizing the adequacy of monitor locations
- Plots (graphs) of potential emissions levels and/or historical monitored levels of pollutants versus monitor locations
- Modeling or special studies (including saturation monitoring studies) may be appropriate for determining the adequacy of a particular monitor location

3 Idaho DEQ's Ambient Air Monitoring Network

DEQ is responsible for operating and maintaining the ambient air monitoring network for the State of Idaho. Some air monitors in Idaho are managed by tribal monitoring organizations on tribal lands. This document is limited to the monitors in the air monitoring network that are managed by DEQ (Figure 1).

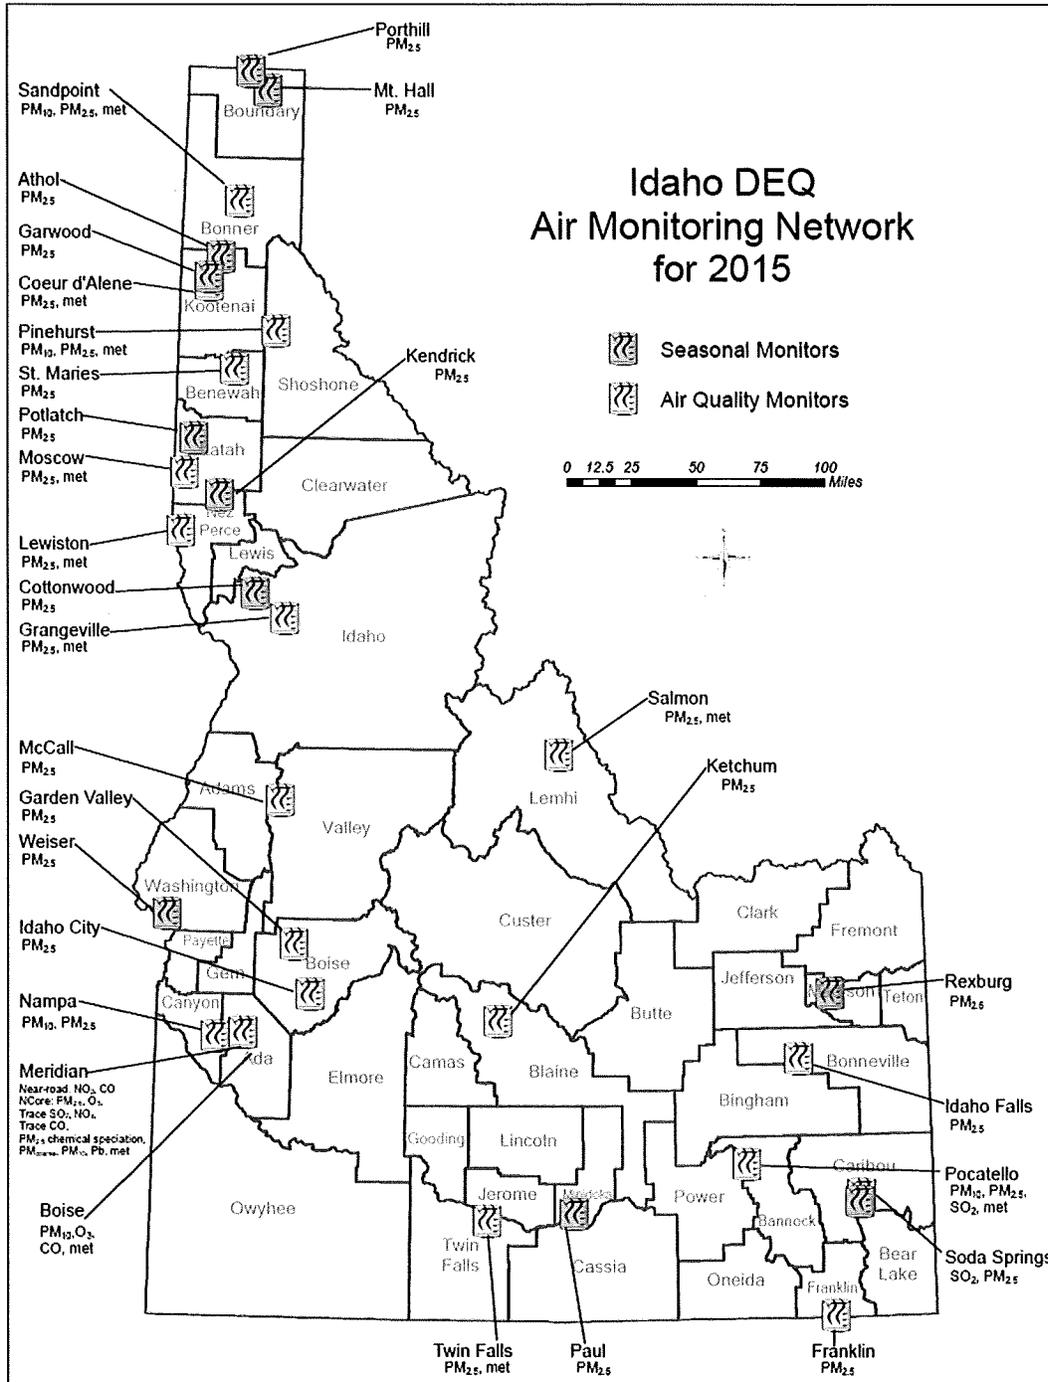


Figure 1. Idaho air quality monitoring network, 2015.

3.1 Monitoring Sites

On January 1, 2015, DEQ’s SLAMS air monitoring network consisted of 28 distinct monitoring sites measuring criteria pollutants and surface meteorology (Table 1). DEQ’s ambient air monitoring network is operated and maintained by monitoring staff at DEQ’s six regional offices.

Table 1. DEQ monitoring stations, locations, and AQS identification codes.

Site	Address	Latitude/ Longitude	AQS Identification
Sandpoint– University of Idaho	U of I Research Center, 2105 N. Boyer Ave. Sandpoint, ID 83864	+48.291820/ - 116.556560	160170003
Coeur d'Alene– Lancaster Rd.	Lancaster Road Hayden, ID 83835	+47.788908/ -116.804539	160550003
Coeur d'Alene LMP	Camp Cross, McDonald Point Lake Coeur d'Alene, ID	+47.555253/ -116.817331	160550004
St. Maries	Forest Service Building St. Maries, ID 83666	+47.316667/ -116.570280	160090010
Pinehurst	106 Church St. Pinehurst, ID 83850	+47.536389/ -116.236667	160790017
Moscow	1025 Plant Sciences Rd. Moscow, ID 83843	+46.728000/ -116.955667	160570005
Lewiston	1200 29th St. Lewiston, ID 83501	+46.408352/ -116.992533	160690012
Grangeville	US Forest Service Compound Grangeville, ID 83530	+45.9274167/ -116.105944	160490002
McCall	500 N. Mission St. McCall, ID 83638	+44.542486/ -116.062358	160850002
Garden Valley	946 Banks Lowman Rd. Garden Valley, ID 83622	+44.104675/ -115.973084	160150002
Nampa	923 1st St S. Nampa, ID 83651	+43.580310/ -116.562676	160270002
Meridian– St. Luke's	Eagle Rd & I-84 Meridian, ID 83642	+43.600699/ -116.347853	160010010
Meridian– Near-road	1311 East Central Dr. Meridian, ID 83642	+43.593929/ -116.38125	160010023
Boise– Eastman Garage	166 N. 9th Boise, ID 83702	+43.616379/ -116.203817	160010014
Boise– Fire Station #5	16th & Front Boise, ID 83702	+43.618889/ -116.213611	160010009
Boise– White Pine Elementary	401 East Linden St. Boise, ID 83706	+43.577603/ -116.178156	160010017
Garden City	Ada County Fairgrounds Garden City, ID 83714	+43.647819/ -116.269514	160010020
Idaho City	3851 Hwy 21 Idaho City, ID 83631	+43.823017/ -115.838557	160150001
Ketchum	111 West 8th St. Ketchum, ID 83340	+43.682558/ -114.371094	160130004
Twin Falls	650 W. Addison Twin Falls, ID 83301	+42.56505/ -114.494767	160830007
Kimberly	50 Highway 50 Kimberly, ID 83341	+42.553325/ -114.354853	160830009
Pocatello	Garrett & Gould Pocatello, ID 83204	+42.876725/ -112.460347	160050015

Site	Address	Latitude/ Longitude	AQS Identification
Pocatello– Sewage Treatment Plant	Batiste Chubbuck Rd. Pocatello, ID 83204	+42.916389/ -112.515833	160050004
Franklin	East 4800 South Road Franklin, ID 83237	+42.013333/ -111.809167	160410001
Soda Springs	5-Mile Rd. Soda Springs, ID 83276	+42.695278/ -111.593889	160290031
Idaho Falls	Hickory and Sycamore St. Idaho Falls, ID 83402	+43.464700/ -112.046450	160190011
Salmon– Charles St.	N. Charles St. Salmon, ID 83467	+45.181893/ -113.890285	160590004
Salmon– Hwy 93	0.8 miles south of Hwy 93/48 intersection Salmon, ID 83468	+45.161682/ -113.892212	160590005

DEQ also uses seasonal monitors at 11 locations for the state’s Crop Residue Burning (CRB) Program (Table 2). The seasonal duration these monitors run varies widely, as they are operated on a case-by-case basis.

Table 2. CRB station locations.

Site	Address	Latitude/ Longitude
Porthill	Tavern Farm Rd. Porthill, ID 83853	+48.995911/ -116.509953
Mt. Hall	1275 Idaho 1 Bonners Ferry, ID 83805	+48.894014/ -116.359381
Athol	NE corner of Pastime St./Grove Ave. Athol, ID 83801	+47.948925/ -116.710978
Garwood	17506 N. Ramsey Rd. Rathdrum, ID 83858	+47.830706/ -116.806794
Cottonwood	BLM Field Office, 1 Butte Dr. Cottonwood, ID 83522	+46.06319/ -116.34824
Potlatch	510 Elm St. Potlatch, ID 83855	+46.92106/ -116.89627
Kendrick	Kendrick Pump Station Kendrick, ID 83537	+46.61291/ -116.659278
Weiser	690 W. Indianhead Rd. Weiser, ID 83672	+44.261694/ -116.979172
Paul	201 N. 1st Street West Paul, ID 83347	+42.6078167/ -113.7868167
Soda Springs	Caribou Hospital, 300 South 3rd Street West Soda Springs, ID 83276	+42.651670/ -111.614720
Rexburg	Madison Middle School, 575 W. 7th Street Rexburg, ID 83440	+43.809486/ -111.800475

3.2 DEQ Monitoring Network—Monitoring Purpose, Scale of Representativeness, and Area Represented

The ambient air quality and meteorological data collected from DEQ's network is used for a variety of purposes, including the following:

- Determining compliance with the NAAQS
- Determining the locations of maximum pollutant concentrations
- Forecasting air quality to determine the AQI
- Providing for early detection of smoke impacts (smoke management)
- Determining the effectiveness of air pollution control programs
- Evaluating the effects of air pollution levels on public health
- Tracking the progress of air quality-related SIPs
- Supporting pollutant dispersion models
- Developing responsible, cost-effective air pollution control strategies
- Analyzing air quality trends

The concept of spatial scale of representativeness is used to clarify the link between general monitoring objectives, site types, and the physical location of a particular monitor. The goal in locating monitors is to correctly match the spatial scale represented by the sample of monitored air with the spatial scale most appropriate for the monitoring site type, the air pollutant measured, and the monitoring objective. Thus, spatial scale of representativeness is described in terms of the physical dimensions of the air parcel nearest to a monitoring site throughout which actual pollutant concentrations are reasonably similar. The scales of interest for the monitoring site types described above are as follows:

1. **Microscale**—Defines the concentrations in air volumes associated with area dimensions ranging from several meters up to about 100 meters.
2. **Middle scale**—Defines the concentrations typical of areas up to several city blocks in size with dimensions ranging from about 100 to 500 meters.
3. **Neighborhood scale**—Defines concentrations within some extended area of the city that has relatively uniform land use with dimensions in the range of 0.5–4.0 kilometers.
4. **Urban scale**—Defines concentrations within an area of city-like dimensions, on the order of 4–50 kilometers. Within a city, the geographic placement of emissions sources may result in no single site that can be said to represent air quality on an urban scale. The neighborhood and urban scales have the potential to overlap in applications that concern secondarily formed or homogeneously distributed air pollutants.
5. **Regional scale**—Defines an area that is usually rural, is of reasonably homogeneous geography without large emissions sources, and extends from tens to hundreds of kilometers.
6. **National and global scales**—These measurement scales represent concentrations characterizing a nation or the globe as a whole.

Proper siting of a monitor requires specifying the monitoring objective, the types of sites necessary to meet the objective, and the desired spatial scale of representativeness. For example, consider a case where the objective is to determine NAAQS compliance by understanding the

maximum ozone concentrations for an area. Candidate areas would most likely be located downwind of a metropolitan area, probably in suburban residential areas where children and other susceptible individuals are likely to be outdoors. Sites in such areas are most likely to represent an urban scale of measurement. In this example, physical location would be determined by considering ozone precursor emission patterns, public activity, and meteorological characteristics affecting ozone formation and dispersion. Thus, spatial scale of representativeness would not be used in the selection process but would be a result of site location.

In some cases, the physical location of a site is determined from jointly considering both the basic monitoring objective and the type of monitoring site desired or required. For example, to determine typical PM_{2.5} concentrations over a geographic area that has relatively high PM_{2.5} concentrations, a neighborhood scale site is most appropriate. Such a site would likely be located in a residential or commercial area having a high overall PM_{2.5} emission density but not in the immediate vicinity of any single dominant source. In this example, the desired scale of representativeness would be an important factor in determining the physical location of the monitoring site.

In either case, classification of the monitor by its type and spatial scale of representativeness is necessary and will aid in interpreting the monitoring data for a particular monitoring objective (e.g., public reporting, NAAQS compliance determination, or research support).

Table 3 illustrates the relationship between the various site types that can be used to support the three basic monitoring objectives and the scales of representativeness that are generally most appropriate for each site type.

Table 3. Relationships between site types and scales of representativeness.

Site Type	Appropriate Siting Scales
Maximum concentration	Micro, middle, neighborhood (<i>sometimes</i> urban or regional for secondarily-formed pollutants)
Population oriented	Neighborhood, urban.
Source impact	Micro, middle, neighborhood
General/background	Urban, regional
Regional transport	Urban, regional
Welfare-related impacts	Urban, regional

Federal ambient air monitoring regulations use the statistical-based definitions for metropolitan areas provided by the Office of Management and Budget and the Census Bureau. These areas are referred to as metropolitan statistical areas or micropolitan statistical areas—both of which are core-based statistical areas (CBSA)—and combined statistical areas (CSA). A CBSA associated with at least one urbanized area of 50,000 population or greater is termed a metropolitan statistical area. A CBSA associated with at least one urbanized cluster of at least 10,000 population or greater is termed a micropolitan statistical area. A CSA consists of two or more adjacent CBSAs. The term MSA is used to refer to a metropolitan statistical area.

By definition, both MSAs and CSAs have a high degree of integration; however, many such areas cross state or other political boundaries. An MSA or CSA may also cross more than one

airshed. EPA recognizes that state or local agencies must consider MSA/CSA boundaries and their own political boundaries and geographical characteristics in designing their air monitoring networks. EPA also recognizes there may be situations where the EPA regional administrator and the affected state or local agencies may need to augment or to divide the overall MSA/CSA monitoring responsibilities and requirements among these various agencies to achieve an effective network design. Full monitoring requirements apply separately to each affected state or local agency in the absence of an agreement between the affected agencies and the EPA regional administrator.

Table 4 summarizes the monitoring purpose, area represented, and monitoring scale of representativeness for DEQ's monitoring sites, including seasonal monitors.

Table 4. Monitoring objectives, areas represented, and scales of representation.

Site	Monitoring Objective	Area Represented	Monitoring Scale
Sandpoint— University of Idaho	AQI, PM ₁₀ SIP, PM ₁₀ NAAQS, smoke management, modeling-meteorological	Bonner County	Urban
Coeur d'Alene— Lancaster Rd.	AQI, smoke management, modeling-meteorological	Coeur d'Alene, ID MSA	Urban
Coeur d'Alene—LMP	Modeling-meteorological	Coeur d'Alene, ID MSA	Neighborhood
St. Maries	PM _{2.5} NAAQS, AQI, smoke management	Benewah County	Neighborhood
Pinehurst	PM ₁₀ SIP, PM ₁₀ NAAQS, PM _{2.5} NAAQS, AQI, smoke management, modeling-meteorological	Shoshone County	Neighborhood
Porthill	Smoke management	Boundary County	Urban
Mt. Hall	Smoke management	Boundary County	Urban
Athol	Smoke management	Kootenai County	Urban
Garwood	Smoke management	Kootenai County	Urban
Moscow	AQI, smoke management, modeling-meteorological	Latah County	Neighborhood
Lewiston	AQI, smoke management, modeling-meteorological	Lewiston ID–WA MSA	Neighborhood
Grangeville	AQI, smoke management, modeling-meteorological	Idaho County	Neighborhood
Cottonwood	Smoke management	Idaho County	Neighborhood
Potlatch	Smoke management	Latah County	Neighborhood
Kendrick	Smoke management	Latah County	Neighborhood
McCall	AQI, smoke management	Valley County	Neighborhood
Garden Valley	AQI, smoke management	Boise County	Neighborhood
Nampa	PM ₁₀ NAAQS, PM _{2.5} NAAQS, AQI	Boise City–Nampa MSA ^a	Neighborhood

Site	Monitoring Objective	Area Represented	Monitoring Scale
Meridian— St. Luke's	NCore—trace gas, NCore— PM _{10-2.5} , PM _{2.5} NAAQS, PM _{2.5} chemical speciation, O ₃ NAAQS, Pb NAAQS, AQI, modeling-meteorological	Boise City–Nampa MSA ^a	Neighborhood
Meridian— Near-road	NO, NO ₂ , NO _x , CO	Boise City–Nampa MSA ^a	Micro
Boise— Eastman Garage	CO SIP, CO NAAQS	Northern Ada County	Micro
Boise— Fire Station #5	PM ₁₀ SIP, PM ₁₀ NAAQS	Northern Ada County	Neighborhood
Boise— White Pine Elementary	O ₃ NAAQS	Boise City–Nampa MSA ^a	Neighborhood
Garden City	Modeling-meteorological	Boise City-Nampa MSA ^a	Neighborhood
Idaho City	Smoke management, AQI	Boise County	Neighborhood
Weiser	Smoke management	Washington County	Neighborhood
Ketchum	Smoke management, AQI	Blaine County	Urban
Twin Falls	Smoke management, AQI	Twin Falls, ID micropolitan statistical area	Neighborhood
Kimberly	Modeling-meteorological	Twin Falls, ID micropolitan statistical area	Urban
Paul	Smoke management	Minidoka County	Neighborhood
Pocatello— Garrett and Gould	PM ₁₀ SIP, PM ₁₀ NAAQS, AQI, modeling-meteorological	Pocatello, ID MSA	Neighborhood
Pocatello— Sewage Treatment Plant	SO ₂ NAAQS	Pocatello, ID MSA	Middle
Franklin	PM _{2.5} NAAQS, AQI	Logan UT–ID MSA	Urban
Soda Springs	SO ₂ NAAQS	Caribou County	Micro - Middle
Soda Springs— Caribou Hospital	Smoke management	Caribou County	Urban
Idaho Falls	AQI	Idaho Falls, ID MSA	Neighborhood
Salmon— Charles St.	PM _{2.5} NAAQS, AQI	Lemhi County	Neighborhood
Salmon— Hwy 93 ^b	Modeling-meteorological	Lemhi County	Urban
Rexburg	Smoke management	Madison County	Urban

Note: AQI – air quality index; SIP – state implementation plan; NAAQS – national ambient air quality standard; PM₁₀ – particulate matter less than 10 microns in diameter; MSA – metropolitan statistical area; O₃ – ozone; PM_{2.5} – particulate matter less than 2.5 microns in diameter; NO – nitric oxide, NO₂ – nitrogen dioxide, NO_x – nitrogen oxides; SO₂ – sulfur dioxide; Pb – Lead; CO – carbon monoxide

^a Boise City–Nampa MSA, as defined by the US Census Bureau, includes Ada, Boise, Canyon, Gem, and Owyhee Counties.

^b The meteorological tower from this location will be moved to the Salmon Charles St. site in 2015.

3.3 Monitoring Methods, Monitor Designation, and Sampling Frequency

Monitoring methods used for making NAAQS compliance determinations at a SLAMS site must be designated FRM or FEM in accordance with 40 CFR Part 53. A method for monitoring PM_{2.5} concentrations that has not been designated as an FRM or FEM may be approved as an ARM by the EPA regional administrator. SPMs do not meet any of the above criteria and are typically used for special studies or as surrogate measures or indicators of emergency episodes (e.g., tapered element oscillating microbalance (TEOM) monitors used for early detection of smoke).

Table 5 lists monitoring methods used by DEQ along with associated method codes required when submitting the monitoring data to EPA's AQS database. Method codes for meteorological parameters are not included in the table.

Table 5. Air monitoring method codes.

Parameter/ Pollutant ^a	Method Designation ^b	AQS Method Code	Instrument and Instrument Parameters
PM ₁₀	FEM	079	TEOM—gravimetric analysis, instrumental—R&P SA246B inlet
CO	FRM	593 ^c	Teledyne API Model 300EU
	FEM	593	Teledyne API Model T300U
	FEM	093	Teledyne API Model T300
SO ₂	FEM	100	Teledyne API Model T100—UV fluorescent
	FEM	060	Thermo Model 43C, pulsed fluorescence
	FRM	600 ^c	Teledyne API Model 100EU—UV fluorescent
O ₃	FEM	087	Teledyne API, Model 400E
	FEM	087	Teledyne API Model T400
NO ₂	FRM	099	Teledyne API, Model 200E—chemiluminescence
	FEM	200	Teledyne API Model T200UP—Photolytic
	FEM	599	Teledyne API, Model 200EU
NO _y	FEM	599 ^c	Teledyne API, Model 200EU
PM _{2.5}	FRM	145	R&P Model 2025 sequential w/ VSCC
PM _{2.5}	SPM	701 or 703 ^d	R&P TEOM w/ SCC—no correction factor
	SPM	715 or 716 ^d	R&P TEOM w/ VSCC—no correction factor
	SPM	178	Thermo TEOM 1405 w/ SCC
	FEM	581	Thermo TEOM 1405-F (FDMS) w/ VSCC
	SPM	183	Thermo TEOM 1405-F (FDMS) w/ SCC
	FEM	170	Met One Beta Gauge (BAM) w/ VSCC
	SPM	731	Met One Beta Gauge (BAM) w/ SCC
PM _{10-2.5}	FRM	176	Thermo Scientific Partisol-Plus Model 2025 Sequential Sampler Pair w/ VSCC
PM ₁₀ Pb	FEM	811	Thermo/R & P 2025 PM10 w/ VSCC w/ XRF analysis

Notes: VSCC – very sharp cut cyclone; SCC – sharp cut cyclone; TEOM – tapered element oscillating microbalance; FDMS – filter dynamics measurement system; BAM – beta attenuation monitor

^a PM₁₀ – particulate matter less than 10 microns in diameter; CO – carbon monoxide; SO₂ – sulfur dioxide; O₃ – ozone; NO₂ – nitrogen dioxide; NO_y – total reactive nitrogen; PM_{2.5} – particulate matter less than 2.5 microns in diameter; PM_{10-2.5} – particulate matter in between 2.5 and 10 microns in diameter; PM₁₀-Pb – Lead

^b FEM – federal equivalent method; FRM – federal reference method; SPM – special purpose monitor

^c Trace gas monitor – NCore

^d Applicable code varies seasonally w/ instrument operating temperature settings

Monitoring sites designated as SLAMS are intended to address specific air quality management interests and are frequently single-pollutant measurement sites. The SLAMS sites must be approved by the EPA regional administrator.

Monitoring sites designated as SPMs in the annual network plan and in the AQS do not count toward meeting network minimum requirements. SPM sites using methods designated as FRMs or FEMs or approved as ARMs are bound to the quality assurance requirements of 40 CFR Part 58 Appendix A.

Gaseous pollutants and meteorological parameters are sampled continuously and typically averaged for each hour. Data completeness for a continuous monitor is computed as the number of valid hourly samples collected divided by the number of potential hourly samples for the period in question (e.g., 8,760 potential hourly samples annually).

PM can be sampled continuously or by time-integrated filter-based methods. Filter-based methods typically collect samples for 24-hour periods. For NAAQS comparison, PM data are reported as a 24-hour average, collected from midnight to midnight at local standard time. The minimum monitoring schedule for a PM_{2.5} site is based on the type of monitor, the monitor's objectives, and the design value (relative to the 24-hour NAAQS) determined for the monitored site (Figure 2).

For the monitors in DEQ's ambient air quality monitoring network, Table 6 lists a variety of parameters associated with the monitors as well as information that is used in reporting data to AQS.

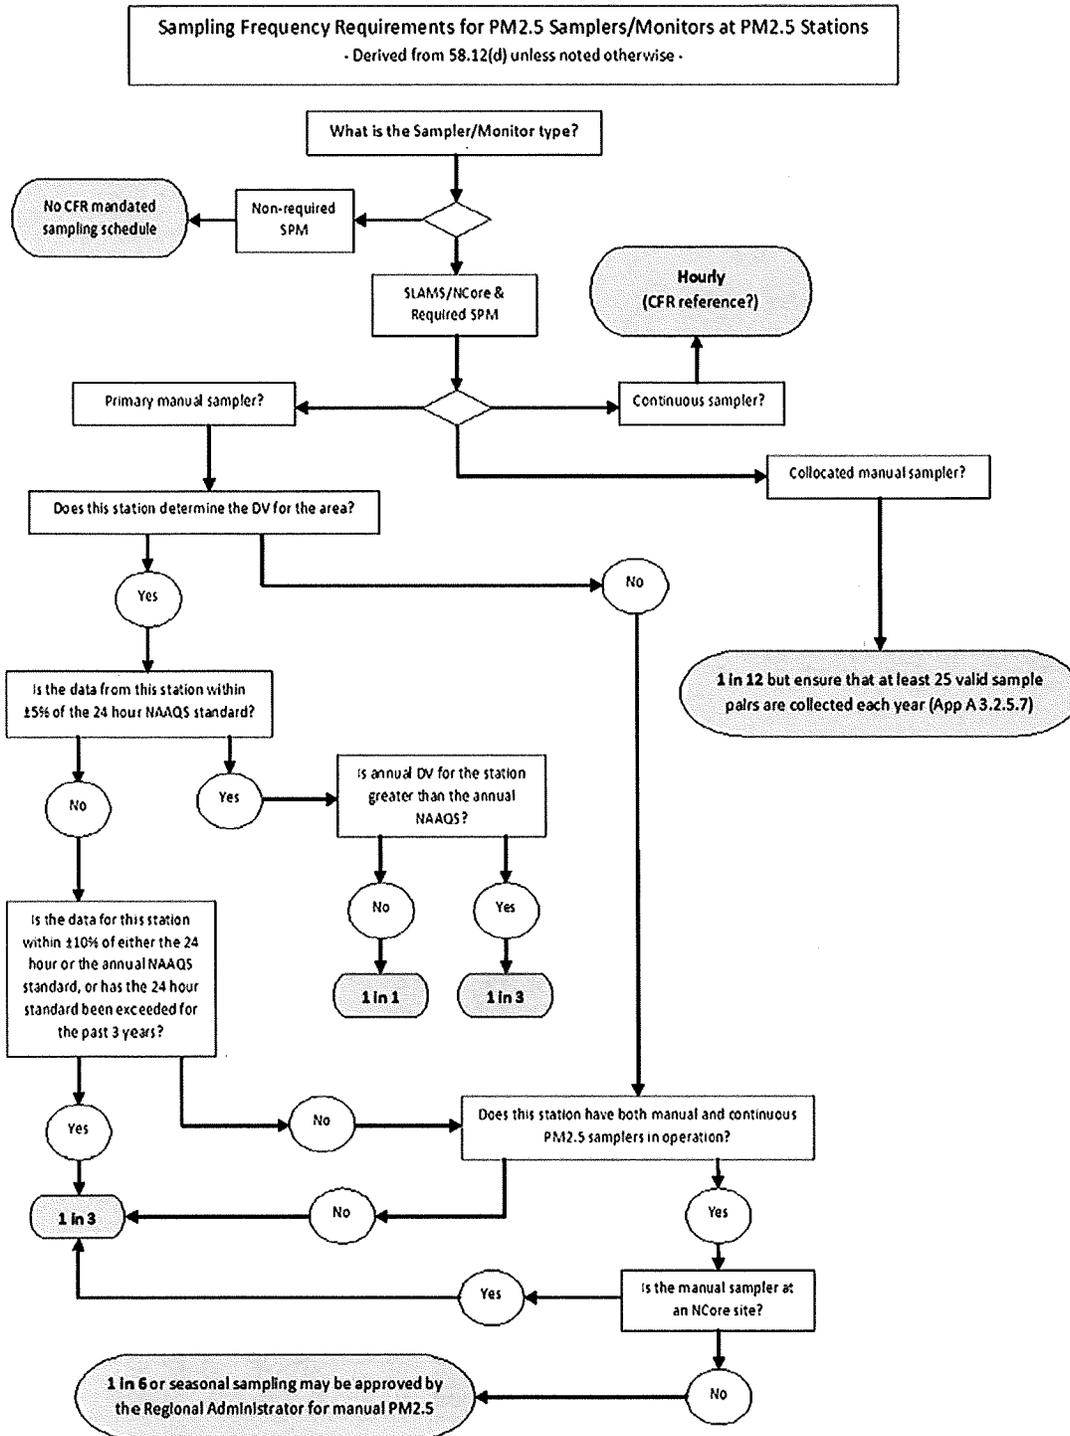


Figure 2. Minimum monitoring frequency based on ratio of local concentration to standard. (Note: DV = design value.)

Table 6. Site summary including pollutants monitored, monitor designation, monitoring frequency, and method codes.

Site	Pollutant Monitored	Begin Date	Monitor Designation	Monitoring Frequency	AQS Method Code	Parameter Code	POC #
Sandpoint— University of Idaho	10-meter meteorology	2013	SPM	Continuous	— ^a	— ^a	— ^a
	PM ₁₀ —TEOM	2013	SLAMS	Continuous	079	81102	3
	PM _{2.5} —BAM 1020	2015	SPM	Continuous	731	88502	3
Coeur d'Alene— Lancaster Rd.	PM _{2.5} —BAM 1020	2015	SPM	Continuous	731	88502	3
	10-meter meteorology		SPM	Continuous	— ^a	— ^a	— ^a
Coeur d'Alene LMP	10-meter meteorology		SPM	Continuous	— ^a	— ^a	— ^a
St. Maries	PM _{2.5} —FRM	2003	SLAMS	1/6	145	88101	1
	PM _{2.5} —BAM 1020	2014	SPM	Continuous	731	88502	3
Pinehurst	PM _{2.5} —FRM	1999	SLAMS	1/1	145	88101	1
	PM _{2.5} —BAM 1020	2014	SLAMS	Continuous	170	88101	3
	PM ₁₀ —TEOM	1998	SLAMS	Continuous	079	81102	3
	10-meter meteorology		SPM	Continuous	— ^a	— ^a	— ^a
Moscow	PM _{2.5} —TEOM	2001	SPM	Continuous	715 or 716	88502	3
	10-meter meteorology		SPM	Continuous	— ^a	— ^a	— ^a
Lewiston	PM _{2.5} —TEOM	2001	SPM	Continuous	715 or 716	88502	3
	10-meter meteorology		SPM	Continuous	— ^a	— ^a	— ^a
Grangeville	PM _{2.5} —TEOM	2000	SPM	Continuous	715 or 716	88502	3
	10-meter meteorology		SPM	Continuous	— ^a	— ^a	— ^a
McCall	PM _{2.5} —TEOM	2010	SPM	Continuous	715 or 716	88502	3
Garden Valley	PM _{2.5} —TEOM	2001	SPM	Continuous	715 or 716	88502	3
Nampa	PM ₁₀ —TEOM	2000	SLAMS	Continuous	079	81102	2
	PM _{2.5} —FRM	2008	SLAMS	1/6	145	88101	1
	PM _{2.5} —BAM 1020	2015	SPM	Continuous	731	88502	3

Site	Pollutant Monitored	Begin Date	Monitor Designation	Monitoring Frequency	AQS Method Code	Parameter Code	POC #
Meridian— St. Luke's	PM _{2.5} —FRM	2006	NCORE	1/3	145	88101	1
	PM _{2.5} 1405-F TEOM/FDMS	2015	SPM	Continuous	183	88502	3
	PM _{2.5} Chemical Speciation	2006	NCORE	1/3	810	88502	5
	PM _{10-2.5}	2011	NCORE	1/3	176	86101	1
	O ₃	2007	NCORE	Continuous	087	44201	1
	SO ₂	2009	NCORE	Continuous	600	42401	1&2
	NO _y	2009	NCORE	Continuous	599	42600/42601/42612	1,3,1
	CO	2009	NCORE	Continuous	593	42101	1
	PM ₁₀ Pb	2011	NCORE	1/6	811	85129	1
	10-meter meteorology		NCORE	Continuous	— ^a	— ^a	— ^a
	PM _{2.5} —FRM	2013	Precision	1/6	145	88101	2
	PM ₁₀ Pb	2011	Precision	1/12	811	85129	2
Meridian— Near-road	NO ₂ ,NO,NO _x (Photolytic)	2012	SLAMS/Near-road	Continuous	200	42602/42601/42603	1,1,1
	CO	2012	SLAMS/Near-road	Continuous	593	42101	1
Boise— Eastman Garage	CO	1993	SLAMS	Continuous	093	42101	1
Boise— Fire Station #5	PM ₁₀ —TEOM	1999	SLAMS	Continuous	079	81102	3
Boise— White Pine Elementary	O ₃	2009	SLAMS	Continuous	087	44201	1
Garden City	10-meter meteorology		SPM	Continuous	— ^a	— ^a	— ^a
Idaho City	PM _{2.5} —TEOM	2000	SPM	Continuous	715 or 716	88502	3
Ketchum	PM _{2.5} —TEOM (seasonal)	2009	SPM	Continuous	715 or 716	88502	3
Twin Falls	PM _{2.5} —1405 TEOM	2015	SPM	Continuous	178	88502	4
Kimberly	10-meter meteorology		SPM	Continuous	— ^a	— ^a	— ^a

Site	Pollutant Monitored	Begin Date	Monitor Designation	Monitoring Frequency	AQS Method Code	Parameter Code	POC #
Pocatello	PM _{2.5} —TEOM	2002	SPM	Continuous	715 or 716	88502	3
	PM ₁₀ —TEOM	2001	SLAMS	Continuous	079	81102	3
	10-meter meteorology		SPM	Continuous	— ^a	— ^a	— ^a
Pocatello— Sewage Treatment Plant	SO ₂	1981	SLAMS	Continuous	100	42401	2&4
Franklin	PM _{2.5} —FRM	2004	SLAMS	1/3	145	88101	1
	PM _{2.5} 1405-F TEOM/FDMS	2013	SPM	Continuous	183	88502	3
	PM _{2.5} —BAM 1020	2015	SPM	Continuous	731	88502	3
Soda Springs	SO ₂	2000	SLAMS	Continuous	100	42401	1&2
Idaho Falls	PM _{2.5} —BAM 1020	2015	SPM	Continuous	731	88502	4
Salmon— Charles St.	PM _{2.5} —FRM	2003	SLAMS	1/3	145	88101	1
	PM _{2.5} —BAM 1020	2009	SPM	Continuous	731	88502	3
Salmon— Hwy 93	10-meter meteorology		SPM	Continuous	— ^a	— ^a	— ^a

Note: PM₁₀ – particulate matter less than 10 microns in diameter; PM_{2.5} – particulate matter less than 2.5 microns in diameter; TEOM – tapered element oscillating microbalance; O₃ – ozone; NO₂ – nitrogen dioxide; FRM – federal reference method; FDMS – filter dynamics measurement system; BAM – beta attenuation monitor; SO₂ – sulfur dioxide; NO – nitric oxide; NO_x – nitrogen oxides; NO_y – total reactive nitrogen; CO – carbon monoxide; PM_{10-2.5} – particulate matter in between 2.5 and 10 microns in diameter;

Pb – Lead

^a Meteorological parameters are listed in Table 7.

DEQ currently operates twelve 10-meter meteorological stations. Meteorological measurements are used to support AQI forecasting and air quality modeling analyses. Data collected from DEQ's meteorological stations are submitted to AQS.

Table 7 provides a list of parameters measured at DEQ meteorological stations. DEQ operates the meteorological monitoring network in accordance with EPA's *Quality Assurance Handbook for Air Pollution Measurement Systems Volume IV: Meteorological Measurements Version 2.0 (Final)* (2008).

Table 7. DEQ meteorological monitoring stations and parameters.

Site	Meteorological Parameters Monitored							
	2-meter temp. (°C)	10-meter temp. (°C)	Barometric Pressure (mbar)	Relative Humidity (%)	Wind Direction (degrees)	Wind Speed (m/s)	Solar Radiation (Watt/m ²)	Precipitation (rain, inches)
Sandpoint—University of Idaho	X	X	X	X	X	X	X	X
Pinehurst	X	X	X	X	X	X	X	X
Coeur d'Alene—LMP	X	X	X	X	X	X	X	X
Coeur d'Alene—Lancaster Rd.	X	X	X	X	X	X	X	X
Moscow	X	X	X	X	X	X	X	X
Lewiston	X	X	X	X	X	X	X	X
Grangeville	X	X	X	X	X	X	X	X
Meridian—St. Luke's	X	X	X	X	X	X	X	
Garden City	X	X	X	X	X	X	X	
Kimberly	X	X	X	X	X	X	X	
Pocatello	X	X	X	X	X	X	X	X
Salmon—Hwy 93	X		X	X	X	X	X	

4 DEQ Network Modifications Subsequent to the EPA-Approved 2014 Ambient Monitoring Network Plan

The following network modifications were made after EPA approval of the 2014 ambient monitoring network plan. Modifications proposed/implemented after the 2014 plan and prior to DEQ submitting this 2015 plan have been addressed, case by case, and have been communicated through e-mail and mail, if necessary. Applicable documentation is included in Appendix C.

1. The St. Maries beta attenuation monitor (BAM) 1020 (start date of January 1, 2014) is no longer being tested for FEM comparability. DEQ designated it as an SPM for AQI and smoke management and is continuing to use the FRM at St. Maries as the

- NAAQS monitor. The BAM was converted to an SPM by switching the impactor from a VSCC to an SCC.
2. The Pinehurst and Salmon FRM monitors have been designated the primary NAAQS monitors as of January 1, 2015 (Appendix C). This action was a result of DEQ standardizing its monitoring network where practical, which is a routine goal in all facets of the monitoring network, though not always achievable. The six core SLAMS PM_{2.5} sites all now have FRMs as their primary NAAQS monitors.
 3. The St. Luke's Speciation Air Sampling System monitor PM_{2.5} mass measurement has been discontinued per EPA final ruling since the network already has a PM_{2.5} mass measurement with the FRM monitor at St. Luke's. This change helps to allocate resources elsewhere in the network.

5 Proposed Network Modifications

Below is a brief discussion of DEQ's rationale in proposing network modifications (if any) for each monitored pollutant, followed by a summary of those proposed changes. Annual air quality data summaries for DEQ's air monitoring network can be found at: www.deq.idaho.gov/air-quality/monitoring/monitoring-network. More information about criteria pollutants (those pollutants for which EPA has established NAAQS) and NAAQS can be found at www.epa.gov/air/criteria.

5.1 PM₁₀ Monitoring Network

Five PM₁₀ monitoring sites are currently operating. These monitors support local SIPs and/or PM₁₀ maintenance plans by assessing compliance with the PM₁₀ NAAQS and will continue operating through 2015. PM₁₀ monitoring locations are selected to represent average population exposure to spatially representative concentrations in the middle, neighborhood, and urban scales. The following airsheds are classified as "moderate" nonattainment for the 24-hour PM₁₀ NAAQS (150 micrograms per cubic meter):

- Shoshone County—partial (including the entire city of Pinehurst)
- Fort Hall Reservation (Bannock County—partial, Power County—partial)

The Fort Hall Reservation nonattainment area is on Tribal land and is not administered by DEQ.

The following airsheds were previously classified as nonattainment but are now classified as maintenance areas and require monitoring to demonstrate compliance with a specific PM₁₀ NAAQS over specific timeframes:

- Boise-Northern Ada County
- Bonner County—partial (City of Sandpoint)
- Portneuf Valley (Bannock County—partial, Power County—partial)

PM₁₀ design values for 2012–2014 are listed in Appendix A.

Due to the necessity of PM₁₀ monitoring to meet the regulatory requirements associated with SIPs and maintenance plan objectives, DEQ proposes no substantive change to the PM₁₀ monitoring network.

5.2 PM_{2.5} Core NAAQS Compliance Monitoring Network

DEQ operates a “core network” of six PM_{2.5} monitoring sites for NAAQS compliance. DEQ began monitoring PM_{2.5} by FRM in 1998 with an initial network of 13 sites. Over time, the network has been reduced due to site redundancy within airsheds or overall low ambient concentrations relative to the NAAQS. The following six sites remain:

- Pinehurst
- St. Maries
- Treasure Valley (Nampa—Fire Station)
- Treasure Valley (Meridian—St. Luke’s)
- Salmon
- Franklin

Federal regulations require a minimum of two PM_{2.5} monitoring sites in the Treasure Valley, based on population. The Meridian monitor also satisfies the requirement for PM_{2.5} monitoring at NCore sites.

DEQ is proposing the following changes based on the most recent 2012–2014 24-hour design value:

- The St. Maries FRM’s run schedule is required to change from 1/6 days to 1/1 days, effective no later than January 1, 2016.
- The Nampa Fire Station FRM’s run schedule is required to change from 1/6 days to 1/3 days, effective no later than January 1, 2016.

PM_{2.5} design values (updated for 2012–2014) and current and proposed sampling frequencies are listed in Appendix A. Appendix A Table A2 represents data obtained from both FRM and FEM monitors. Due to FRM filter weighing lab QA/QC issues, 2012–2014 PM_{2.5} FRM data are not comparable to the NAAQS. This limitation applies to the Meridian St. Luke’s, St. Maries, Nampa Fire Station, and Franklin sites. Salmon and Pinehurst were operating FEMs as their primary reporting monitors during 2012–2014, so the data from these sites in the table are comparable to the NAAQS.

5.3 PM_{2.5} Continuous Monitoring Network

DEQ monitors PM_{2.5} year-round (with the exception of Ketchum, which is a seasonal monitor that shuts down during the winter months) at 18 sites throughout the state with continuous PM_{2.5} monitors. The real-time and continuous PM_{2.5} data support DEQ’s air quality forecasting, AQI, and smoke management programs. The BAM 1020 at Pinehurst is also designated a SLAMS monitors for NAAQS compliance assessment, though it is considered secondary to the primary FRM at the site and is only used when the FRM data are unavailable or invalid. The other monitors in the list below are special purpose, non-NAAQS monitors.

The PM_{2.5} continuous monitors are located at these monitoring sites:

- Sandpoint—University of Idaho
- Coeur d’Alene—Lancaster Rd.
- St. Maries

- Pinehurst
- Moscow
- Lewiston
- Grangeville
- McCall
- Garden Valley
- Idaho City
- Nampa
- Meridian —St. Luke’s
- Ketchum (seasonal monitor, shuts down in winter months)
- Twin Falls
- Pocatello
- Franklin
- Idaho Falls
- Salmon

DEQ also uses seasonal SPMs (nephelometers and e-samplers) at 11 locations to support the state’s CRB Program (Table 2).

DEQ is proposing relocating the Franklin 1405-F TEOM to the Pocatello Garrett & Gould site, where its VSCC will be replaced by an SCC making it an SPM for AQI reporting. A BAM 1020 with an SCC, also designated SPM, will be installed in its place at Franklin and used for AQI reporting. The BAM has proven to be easier to maintain, therefore making it practical to place this monitor at a location that requires significant travel time for DEQ staff.

5.4 Ozone Monitoring Network

DEQ currently operates two ozone monitors, both in the Treasure Valley. Federal regulations require two ozone monitors in an urban area or MSA the size of the Boise City–Nampa MSA. One site must be designed to record the maximum concentration for the MSA. NCore sites can be counted toward minimum SLAMS ozone network requirements. Ozone is monitored during the ozone “season” as prescribed in 40 CFR Part 58 Appendix D. For 2015, the ozone season is May 1 through September 30.

The Treasure Valley ozone monitors are located at the following sites:

- The Meridian St. Luke’s NCore site near the Meridian St. Luke’s Hospital
- The White Pine Elementary site in southeast Boise

DEQ began monitoring at the White Pine Elementary school in 2009 when it had to relocate the Whitney Elementary School site, which was demolished in 2008. The White Pine Elementary site was chosen based on evidence that it would represent the maximum ozone concentration for the Boise City–Nampa MSA.

DEQ is proposing no changes to the ozone monitoring network in this 2015 monitoring network plan.

Ozone design values for 2012–2014 are listed in Appendix A.

5.5 Carbon Monoxide (CO) Monitoring Network

Monitoring for carbon monoxide (CO) in the Treasure Valley began in 1977. Violations of the health-based standard for CO occurred every winter from 1977 until 1986, and as a result, Northern Ada County was designated a CO nonattainment area by EPA. In December 2002, the Northern Ada County CO Limited Maintenance Plan was approved by EPA, which reclassified the area as attainment for the CO NAAQS. No exceedances of the CO NAAQS have occurred since 1991.

DEQ operates three CO monitors: one at the Boise–Eastman Garage site in downtown Boise, one at the Meridian St. Luke’s NCore site, and one at the Meridian near-road site. The Boise–Eastman site is an “urban canyon” site designed to measure maximum concentrations to which the population is exposed. This site is needed to demonstrate NAAQS compliance as specified in the Northern Ada County CO Maintenance Plan. The Meridian St. Luke’s CO monitor is a “trace-level” monitor, able to measure much lower CO than conventional CO monitors used for NAAQS compliance. The Meridian St. Luke’s CO monitor is required for NCore sites. The Meridian near-road CO monitor has been established in advance of future EPA requirements for near-road CO monitoring.

CO design values for 2012–2014 for both the 1-hour and 8-hour design values are listed in Appendix A.

DEQ is proposing to relocate the Eastman Garage CO analyzer sampling inlet a minimum of 2 meters from the nearest traffic lane to coincide with recommended siting criteria found in 40 CFR Part 58 Appendix E. If not feasible, DEQ will consider a new site location.

5.6 Sulfur Dioxide (SO₂) Monitoring Network

Three SO₂ monitors currently operate in Idaho:

- Pocatello–Sewage Treatment Plant (STP)
- Soda Springs
- Meridian–St. Luke’s

The Pocatello STP site is a maximum concentration site used to assess impacts of local industrial emissions. The Soda Springs monitor is also a maximum concentration site for assessing industrial impacts from a nearby source. Both SO₂ monitoring locations in southeastern Idaho were identified as fence-line “hot spots” from conventional dispersion model applications. Recently developed wind roses have prompted DEQ to reanalyze siting characteristics of the Soda Springs monitor. This reanalysis will take place in 2015. The St. Luke’s monitor is a “trace-level” monitor required for NCore monitoring.

DEQ is proposing no changes to the SO₂ monitoring network as part of this 2015 monitoring network plan.

SO₂ design values for 2012–2014 are listed in Appendix A.

5.7 Nitrogen Dioxide (NO₂) Monitoring Network

DEQ currently has one SLAMS NO₂ monitoring station at the Meridian near-road site. On January 22, 2010, EPA revised the NO₂ primary NAAQS, along with revisions to the NO₂ monitoring requirements. Per this final rule, Idaho will be required to monitor NO₂ at a “near-road” monitoring station in the Boise City–Nampa MSA. Initially, all monitoring was scheduled to begin January 1, 2013. However, due to funding limitations, EPA has changed the requirement for the Boise City–Nampa MSA (MSA > 500,000) to January 1, 2017. However, prior to the change in implementation date, DEQ received a grant from EPA to pilot a near-road monitoring site, which was established in Meridian approximately 30 meters from Interstate 84. Upon completion of the pilot study (December 31, 2012), DEQ chose to continue NO₂ monitoring at the near-road site in order to sooner assemble a 3-year data record for NAAQS assessment (the NO₂ NAAQS has a 3-year averaging period).

DEQ is proposing no changes to the NO₂ monitoring network as part of this 2015 monitoring network plan.

NO₂ design values for 2012–2014 are listed in Appendix A.

5.8 Lead (Pb) Monitoring Network

On December 14, 2010, EPA made final revisions to the ambient monitoring requirements for measuring lead (Pb). CBSAs with a population of 500,000 people or more were required to initiate lead monitoring at NCore monitoring sites beginning by January 1, 2012. DEQ met this requirement and initiated PM₁₀ lead monitoring at the St. Luke’s NCore site. EPA has also required Pb monitoring near facilities with Pb emissions exceeding 0.5 tons per year (tpy). Idaho has no such facilities and thus is not conducting any source-oriented Pb monitoring.

DEQ is using a low-volume PM₁₀ sampler to collect filter-based samples for lead analysis. A low-volume Partisol 2025 sampler configured to collect PM_{10-2.5} as part of the PM_{10-2.5} (section 5.9) measurement is already collecting PM_{10c} on the every sixth day schedule required for Pb. DEQ is using the National Laboratory Contract and ships the samples/filters to the contract laboratory for PM₁₀-Pb analysis by x-ray fluorescence (XRF) analysis.

Should lead concentrations exceed a 3-month average greater than or equal to 0.1 micrograms per cubic meter, DEQ will be required to install and operate a Pb-TSP monitor within 6 months of such determination. Any PM₁₀-Pb measurements exceeding the NAAQS could lead to a violation of the standard. As of this date, values have been well below this threshold.

Pending final EPA ruling as part of the 40 CFR Part 58 monitoring requirement revisions, DEQ may have the option to discontinue Pb monitoring at its NCore site. If the final monitoring requirement revisions allow for this, DEQ will seek EPA approval to do so, considering that values thus far have been well below the NAAQS.

5.9 PM_{10-2.5} (PM_{coarse})

PM_{10-2.5} (PM_{coarse}) is defined as the particulate fraction with a nominal diameter between 2.5 and 10.0 μ. PM_{10-2.5} is determined by calculating the fractional mass difference between collocated

and matching (i.e., same type of monitor) FRM PM_{10c} and FRM PM_{2.5} monitors. Section 3 of Appendix D, 40 CFR Part 58, requires PM_{10-2.5} monitoring at NCore monitoring stations.

DEQ initiated PM_{10-2.5} monitoring at the Meridian–St. Luke’s NCore site beginning January 1, 2011. Both the PM_{2.5} and PM_{10-2.5} samplers are operated every third day in accordance with the national monitoring schedule. A second PM_{10-2.5} monitor is operated every twelfth day for the purpose of assessing lo-vol PM₁₀ sampling precision.

DEQ is proposing no changes to the PM_{10-2.5} monitoring network as part of this 2015 monitoring network plan.

5.10 Summary of Proposed Network Modifications for DEQ’s 2015 Air Monitoring Network Plan

DEQ is proposing the following network modifications in this plan:

- Change the St. Maries FRM monitor run schedule from 1/6 days to 1/1 days, effective no later than January 1, 2016.
- Change the Nampa Fire Station FRM monitor’s run schedule from 1/6 days to 1/3 days, effective no later than January 1, 2016.
- Pending final EPA ruling as part of 40 CFR Part 58 monitoring requirement revisions, discontinue Pb monitoring at DEQ’s NCore site, upon EPA approval.
- At a minimum, relocate Eastman Garage CO inlet a minimum of 2 meters from nearest traffic lane. If not possible, research moving site to a new location.
- Relocate the Franklin 1405-F TEOM to the Pocatello Garrett & Gould site, where its very sharp cut cyclone (VSCC) will be replaced by a sharp cut cyclone (SCC) making it an SPM for AQI reporting.

6 Future Ambient Air Monitoring Requirements and Associated Costs

EPA is required to review criteria pollutant NAAQS on a routine 5-year schedule. EPA is in the process of completing its review of a number of pollutants and through rulemaking will be proposing changes to ambient air monitoring requirements for some pollutants. This review can result in additional monitors and new monitoring requirements for Idaho. At this time, until rulemakings are made final, it is difficult to specifically project DEQ’s future monitoring requirements and associated costs. DEQ is particularly interested in the ozone NAAQS rulemaking to better assess impacts to the network. This final rulemaking is set to take place October 2015.

This page intentionally left blank for correct double-sided printing.

Appendix A. DEQ Ambient Monitoring Network Design Values

Note: Many of DEQ's PM_{2.5} and PM₁₀ monitors were impacted by smoke from wildfires and dust storms in 2012 and 2013. The Clean Air Act provides for agencies to flag such data for exceptional and natural events and for EPA to concur if appropriate steps and demonstrations are completed. DEQ intends to pursue "exceptional event" exclusion, at a minimum, for Salmon and Pinehurst PM_{2.5} and Boise and Nampa PM₁₀. Design values are provided reflecting inclusion and exclusion of these data. These values are preliminary. DEQ has not determined whether it will seek EPA concurrence for data affecting other monitors because no significant regulatory impact has been determined at this time. This determination is subject to change, depending on what happens in 2015 and 2016.

The PM_{2.5} table below represents data obtained from both FRM and FEM monitors. Due to FRM filter weighing lab QA/QC issues, 2012–2014 PM_{2.5} FRM data are not comparable to the NAAQS for the Meridian–St. Luke's, St. Maries, Nampa Fire Station, and Franklin sites. Salmon and Pinehurst were operating FEMs as their primary reporting monitors during 2012–2014, so the data from these sites in the table below are comparable to the NAAQS.

Table A1. 2012–2014 PM₁₀ design values.

Site	County/ AQS ID	Estimated Exceedances			3-year Estimated Exceedances
		2012	2013	2014	
Sandpoint	Bonner 160170003	0.0	0.0	0.0 ^b	0.0
	160170005 ^a				
Pinehurst	Shoshone 160790017	0.0	1.0/0.0	0.0	0.3/0.0
Nampa	Canyon 160270002	1.0/0.0	0.0 ^b	0.0	0.3/0.0
Boise	Ada 160010009	2.0/0.0	0.0	0.0 ^b	0.7/0.0
Pocatello	Bannock 160050015	2.1/0.0	0.0	0.0	0.7/0.0

Notes: A monitor violates the 24-hour PM₁₀ NAAQS if the 3-year average of estimated exceedances (>150 µg/m³) is greater than 1. Concentration data are denoted with/without exceptional event data included.

^a This site was decommissioned in 2013 and moved to site ID 160170003. A split record exists for 2013 as a result.

^b Monitor did not meet data completeness requirements.

Table A2. 2012–2014 design values for core PM_{2.5} monitoring stations—federal reference or federal equivalent method (primary monitor).

Monitoring Site	County/ AQS ID	98th Percentile 24-hour Concentration (µg/m ³)			2012–2014 24-hour Design Value (µg/m ³)	Required Sampling Frequency ^a (Current Frequency)	2012–2014 Annual Design Value (µg/m ³)
		2012	2013	2014			
Meridian– St. Luke's	Ada 160010010	41/19	89	28/28	53/45	1:3 ^b (1:3)	9.2/8.5
St. Maries	Benewah 160090010	27	35	45/45	36/36	1:1 (1:6)	10.4/10.3
Nampa Fire Station	Canyon 160270002	27/20	50	27/27	35/32 ^c	1:3 (1:6)	Incomplete ^c
Franklin	Franklin 160410001	32/16	55	33/33	40/35	1:3 (1:3)	7.7/7.4
Salmon	Lemhi 160590004	154/34	42	40/40	79/39	1:3 (1:3)	15.6/11.3
Pinehurst	Shoshone 160790017	36/35	43/43	42/42	40/40	1:3 (1:1)	13.0/12.4

Notes: A monitor violates the 24-hour PM_{2.5} NAAQS if the 3-year average of the annual 98th percentile 24-hour average exceeds 35 µg/m³. The annual PM_{2.5} NAAQS is violated if the 3-year average of the annual arithmetic mean exceeds 12 µg/m³. Concentration data are denoted with/without all "flagged" exceptional event data included. The concentration values may change depending on how many of the "flagged" exceptional events are documentable, as concurred by EPA. Special purpose monitors are not listed in this table. Those data are provided in DEQ's annual data summary reports provided on the DEQ webpage.

^a Required sampling frequencies based on flagged exceptional event data excluded. See Figure 2 in the body of the 2015 annual ambient air quality monitoring network plan for an explanation of required monitoring/sampling frequencies.

^b NCore monitors are required to operate every third day.

^c Does not meet data completeness criteria.

Table A3. 2012–2014 O₃ design values.

Site	County/ AQS ID	4th-Highest Daily Maximum 8-hour Average (ppm)			3-year Design Value (ppm)
		2012	2013	2014	
Boise–White Pine	Ada 160010017	0.070	0.074/0.071	0.065	0.069/0.068
Meridian– St. Luke's	Ada 160010010	0.073	0.062	0.062	0.065

Notes: A monitor violates the 8-hour ozone NAAQS if the 3-year average of the annual 4th-highest daily maximum average exceeds 0.075 ppm. Concentration data are denoted with/without exceptional event data included.

Table A4. 2012–2014 CO design values (1-hour).

Site	County/ AQS ID	1st-/2nd-Highest 1-hour Average (ppm)		
		2012	2013	2014
Boise– Eastman	Ada 160010014	23.1/2.3	4.0/3.0	4.7/4.4
Meridian– St. Luke's	Ada 160010010	1.3/1.1	1.2/1.1	1.1/1.1
Meridian– Near-Road	Ada 160010023	2.7/2.6	1.3/1.2	1.3/1.2

Note: A monitor violates the 1-hour CO NAAQS if it exceeds 35 ppm more than once per year.

Table A5. 2012–2014 CO design values (8-hour).

Site	County/ AQS ID	1st-/2nd-Highest 8-hour Average (ppm)		
		2012	2013	2014
Boise– Eastman	Ada 160010014	3.5/1.6	1.7/1.4	2.1/2.1
Meridian– St. Luke's	Ada 160010010	0.9/0.8	0.9/0.9	1.0/0.7
Meridian– Near-Road	Ada 160010023	1.3/1.0	0.9/0.9	0.9/0.8

Note: A monitor violates the 8-hour CO NAAQS if it exceeds 9 ppm more than once per year.

Table A6. 2012–2014 SO₂ design values.

Site	County/ AQS ID	99th Percentile – Highest Daily Maximum 1-hour Average (ppb)			3-year Design Value (ppb)
		2012	2013	2014	
Pocatello– STP	Bannock 160050004	73	40	38	51
Soda Springs	Caribou 160290031	35	31	23	30
Meridian– St. Luke's	Ada 160010010	6	11	5	7

Note: A monitor violates the 1-hour SO₂ NAAQS if the 3-year average of the annual 99th percentile highest daily maximum 1-hour averages exceeds 75 ppb.

Table A7. 2012–2014 NO₂ design values.

Site	County/ AQS ID	98th Percentile – Highest Daily Maximum 1-hour Average (ppb)			3-year Design Value (ppb)
		2012	2013	2014	
Meridian Near-road	Ada 160010023	44	39	43	42

Note: A monitor violates the 1-hour NO₂ NAAQS if the 3-year average of the annual 98th percentile highest daily maximum 1-hour averages exceeds 100 ppb.

This page intentionally left blank for correct double-sided printing.

Appendix B. Craters of the Moon and Hells Canyon Monitoring Stations (Improve Network)

DEQ is leveraging the IMPROVE monitoring network to fulfill requirements for the PM_{2.5} transport (Hells Canyon) and PM_{2.5} background (Craters of the Moon National Monument) monitoring sites (Figure B1).

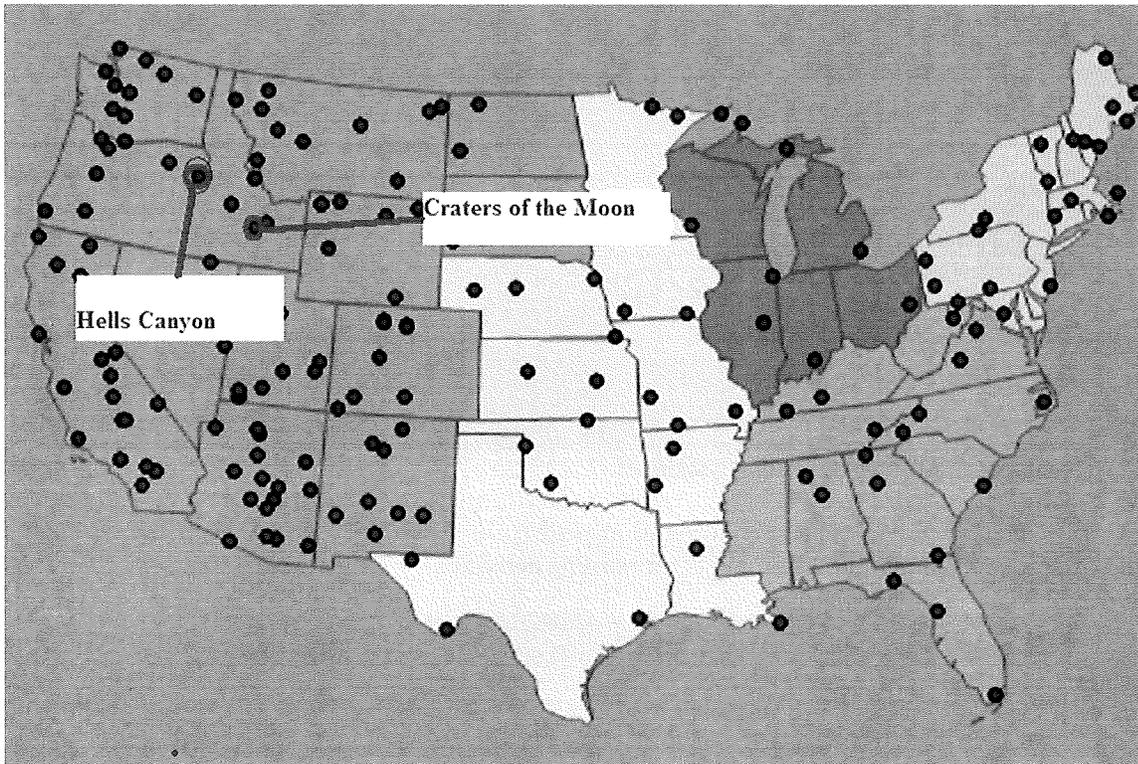


Figure B1. IMPROVE monitoring network.

A history of the IMPROVE monitoring network can be found at: <http://vista.cira.colostate.edu/improve/Default.htm>. The *IMPROVE* program was initiated in 1985 as an extensive long-term monitoring program to establish current visibility conditions, track changes in visibility, and determine causal mechanism for the visibility impairment in national parks and wilderness areas.

Craters of the Moon

Monitoring began at the Craters of the Moon site in 1992 (Figure B2). Metadata for the site can be found at

<http://vista.cira.colostate.edu/improve/Web/Sitebrowser/Sitebrowser.aspx?SiteID=69>. Raw data gathered at this site can be found at <http://views.cira.colostate.edu/web/>.

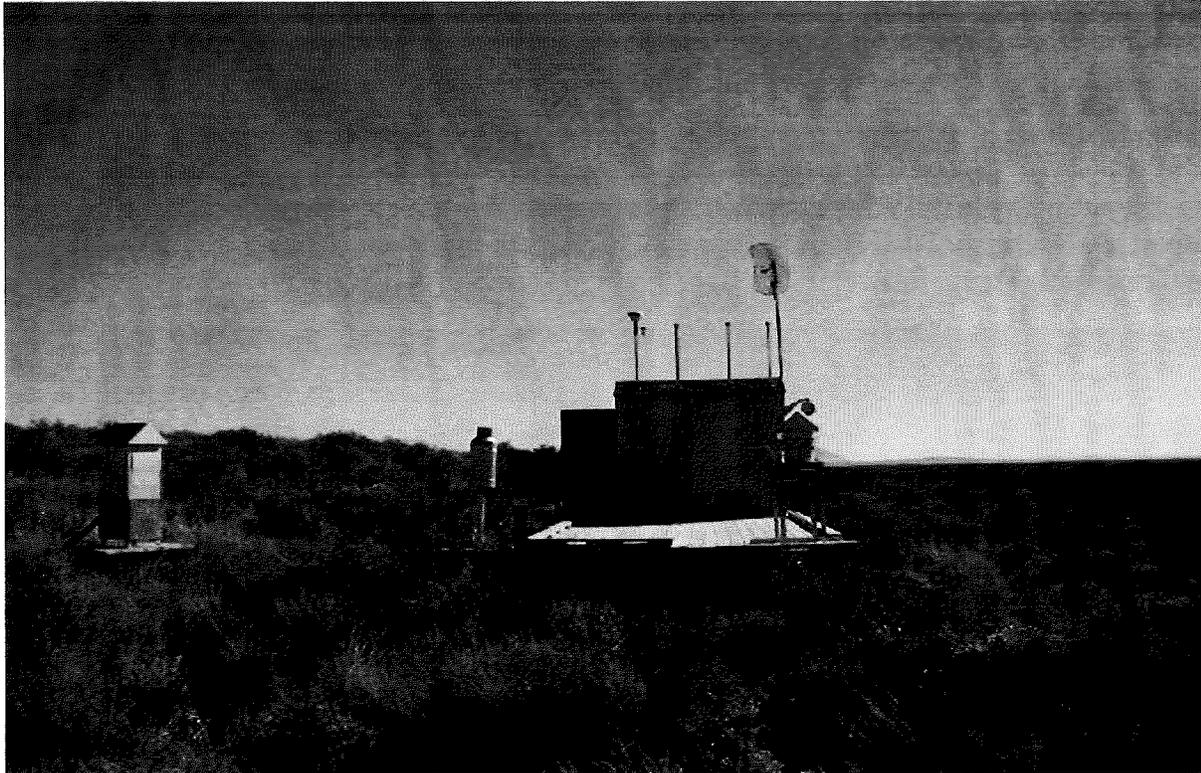


Figure B2. Craters of the Moon sampling platform.

Figure B3 shows the typical background concentration of $PM_{2.5}$ of $1-6 \mu g/m^3$. On occasion, the monitor is impacted by smoke from regional fires and other burning activities.

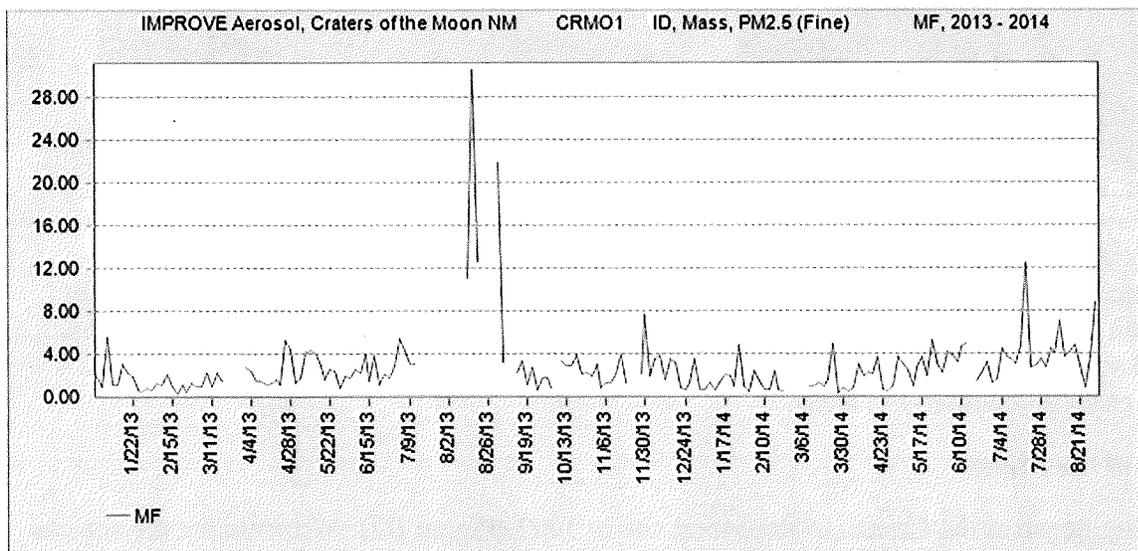


Figure B3. 2013–2014 $PM_{2.5}$ measured at Craters of the Moon IMPROVE site.

Hells Canyon

Monitoring began at the Hells Canyon site in 2001 (Figure B4). Metadata for the site can be found at <http://vista.cira.colostate.edu/improve/Web/Sitebrowser/Sitebrowser.aspx?SiteID=69>. Raw data gathered at this site can be found at <http://views.cira.colostate.edu/web/>.



Figure B4. Hells Canyon monitoring station.

Figure B5 shows the Hells Canyon $PM_{2.5}$ measurements for 2013–2014. Typical transport concentrations of 2–6 $\mu\text{g}/\text{m}^3$ are represented; however, on occasion values can be higher. Typically, elevated levels of $PM_{2.5}$ are associated with either summer/fall smoke impacts or regional winter-time stagnation events.

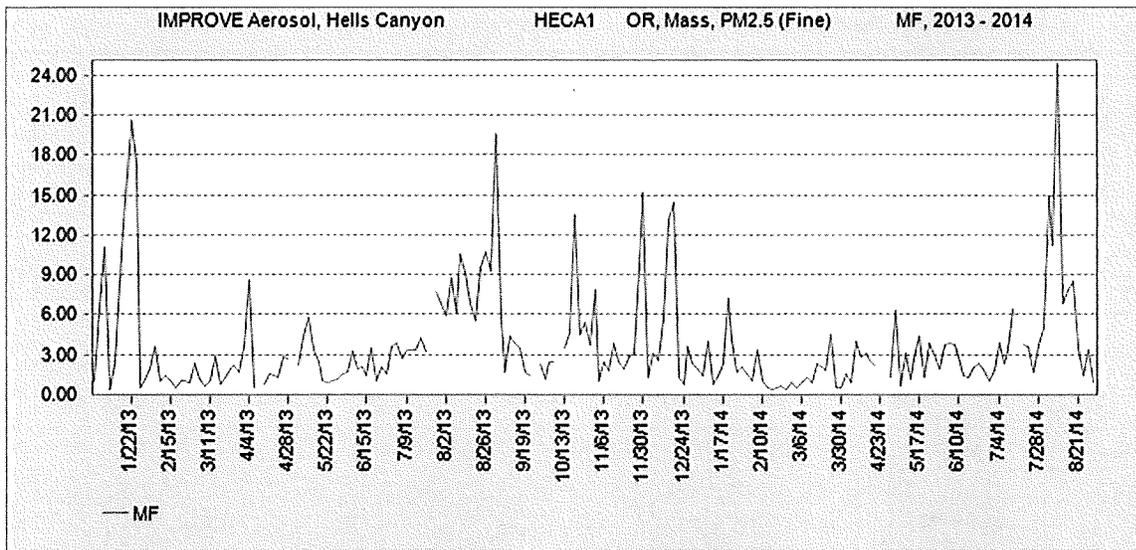


Figure B5. 2013–2014 $PM_{2.5}$ measured at Hells Canyon IMPROVE site.

This page intentionally left blank for correct double-sided printing.

Appendix C. EPA-DEQ Correspondence

This page intentionally left blank for correct double-sided printing.



UNITED STATES ENVIRONMENTAL PROTECTION AGENCY
REGION 10
1200 Sixth Avenue, Suite 900
Seattle, WA 98101-3140

OCT 30 2014

OFFICE OF
AIR, WASTE AND TOXICS

Mr. Bruce Louks
Air Quality Manager
Idaho Department of Environmental Quality
1410 North Hilton
Boise, ID 83706-1255

Dear Mr. Louks:

EPA has evaluated the Idaho Department of Environmental Quality's (DEQ's) 2014 Ambient Air Monitoring Network Plan (2014 Plan). In the 2014 Plan, DEQ proposed changes to its monitoring network. EPA evaluated the proposed changes to the monitoring network in accordance with 40 C.F.R. § 58.10, and with consideration of the applicable requirements of 40 C.F.R. Part 58, Appendices A, C, D and E. Following are EPA's responses to specific proposed network changes:


- DEQ requests EPA to approve a "non-regulatory" designation for two continuous PM_{2.5} Federal Equivalent Monitors (FEM) monitors, specifically the Franklin TEOM 1405-F, and the St. Maries BAM 1020 monitors. The reason for this request is that DEQ would like to evaluate the new TEOM 1405-F and the BAM 1020 monitors further before deciding whether to designate them as primary reporting monitors for these sites. EPA approves the re-designation of these two monitors as non-regulatory since this action would not compromise data collection needed for implementation of a NAAQS, and the collocated PM_{2.5} sampling requirements of Part 58, Appendix A, section 3.2.5 will continue to be met.
- DEQ requests that the Pinehurst and Salmon Federal Reference PM_{2.5} Monitors (FRMs) be designated as the primary monitors at these two locations because the FEMs that are currently designated as the primary reporting monitors at these locations do not correlate well with their collocated FRMs. EPA approves the re-designation of the FRMs as primary monitors at these locations since this action would not compromise data collection needed for implementation of a NAAQS, and the collocated PM_{2.5} sampling requirements of Part 58, Appendix A, section 3.2.5 will continue to be met.

EPA also reviewed the information submitted regarding Idaho's existing monitoring network, and found that the monitoring network generally meets the requirements of 40 C.F.R. Part 58. EPA notes, however, that the Eastman micro-scale CO monitor does not meet minimum roadway intersection and traffic lane distances as specified in Appendix E, section 6.2(b) and (c).

Except for the deficiency noted above regarding the Eastman CO monitor, EPA approves Idaho's 2014 Plan.

If you have any questions about our approval of Idaho's 2014 Plan, please contact Keith Rose at (206) 553-1949.

Sincerely,



Robert Elleman, Acting Manager
Air Planning Unit

cc: Mike McGown, IOO
Keith Rose, OAWT
Chris Hall, OEA
Claudia Vaupel, OAWT

Appendix D. 40 CFR Part 58—Appendix D and E Checklists

This page intentionally left blank for correct double-sided printing.

PART 58 APPENDIX D SITE EVALUATION FORM FOR PM_{2.5}

APPLICABLE SECTION	REQUIREMENT	CRITERIA MET?		
		YES	NO	N/A
4.7.1(a)	States, and where applicable local agencies must operate the minimum number of required PM _{2.5} SLAMS sites listed in Table D-5 of this appendix. Use the form below and Table D-5 to verify if each of your MSAs have the appropriate number of SLAMS FRM/FEM/ARM samplers.	X		
4.7.1(b)	Each required SLAMS FRM/FEM/ARM monitoring stations or sites must be sited to represent area-wide air quality in the given MSA (typically neighborhood or urban spatial scale, though micro-or middle-scale okay if it represent many such locations throughout the MSA).	X		
4.7.1(b)(1)	At least one SLAMS FRM/FEM/ARM monitoring station is to be sited at neighborhood or larger scale in an area of expected maximum concentration for each MSA where monitoring is required by 4.7.1(a).	X		
4.7.1(b)(2)	For CBSAs with a population of 1,000,000 or more persons, at least one FRM/FEM/ARM PM _{2.5} monitor is to be collocated at a near-road NO ₂ station.			X
4.7.1(b)(3)	For MSAs with additional required SLAMS sites, a FRM/FEM/ARM monitoring station is to be sited in an area of poor air quality.	X*		
4.7.2	Each State must operate continuous PM _{2.5} analyzers equal to at least one-half (round up) the minimum required sites listed in Table D-5 of this appendix. At least one required continuous analyzer in each MSA must be collocated with one of the required FRM/FEM/ARM monitors, unless at least one of the required FRM/FEM/ARM monitors is itself a continuous FEM or ARM monitor, in which case no collocation requirement applies.	X		
4.7.3	Each State shall install and operate at least one PM _{2.5} site to monitor for regional background and at least one PM _{2.5} site to monitor regional transport (note locations in comment field). Non-reference PM _{2.5} monitors such as IMPROVE can be used to meet this requirement.	X**		
4.7.4	Each State shall continue to conduct chemical speciation monitoring and analyses at sites designated to be part of the PM _{2.5} Speciation Trends Network (STN).	X		

Comments:

*DEQ has several sites in Idaho that are not found within an officially listed MSA, but DEQ has retained SLAMS FRM/FEM/ARM monitoring stations there due to moderate to poor air quality. Those sites include Pinehurst, Salmon, and St. Maries.

**DEQ uses the IMPROVE network's Hells Canyon site for PM_{2.5} regional transport and the Craters of the Moon National Monument site for PM_{2.5} regional background.

MSA Description ¹	MSA population ^{2,3}	Design Value for years 2012-2014	Minimum required number of PM2.5 SLAMS FRM/FEM/ARM sites (from Table D-5)	Present number of PM2.5 SLAMS FRM/FEM/ARM sites in MSA	Present number of continuous PM2.5 analyzers in MSA	Present number of PM2.5 STN analyzers in MSA
Boise City-Nampa, ID MSA	616,561	8.5 (annual)	2	2	4	2
Logan, UT-ID MSA	125,442	35 (24-hour)	1	1	1	0

¹see http://www2.census.gov/econ/subs/data/msa_codes_2007_to_2011.txt

²Minimum monitoring requirements apply to the metropolitan statistical area (MSA). CBSA includes both MSAs and micropolitan statistical areas.

³Population based on latest available census figures.

MSA population ^{1,2}	Most recent 3-year design value $\geq 85\%$ of any PM2.5 NAAQS ³	Most recent 3-year design value $< 85\%$ of any PM2.5 NAAQS ^{3,4}
>1 million	3	2
500K to 1 million	2	1
50K to <500K ⁵	1	0

¹Minimum monitoring requirements apply to the Metropolitan statistical area (MSA).
²Population based on latest available census figures. <https://www.census.gov/>
³The PM_{2.5} National Ambient Air Quality Standards (NAAQS) levels and forms are defined in 40 CFR part 50.
⁴These minimum monitoring requirements apply in the absence of a design value.
⁵Metropolitan statistical areas (MSA) must contain an urbanized area of 50,000 or more population.

PART 58 APPENDIX D SITE EVALUATION FORM FOR PM10

APPLICABLE SECTION	REQUIREMENT	CRITERIA MET?		
		YES	NO	N/A
4.6(a)	Table D-4 indicates the approximate number of permanent stations required in MSAs to characterize national and regional PM10 air quality trends and geographical patterns. Use the form below and Table D-4 to verify if your PM10 network has to appropriate number of samplers.	X		
Comments:				

MSA Description ¹	MSA population ^{2,3}	Minimum required number of PM10 stations (from Table D-4)	Present number of PM10 stations in MSA
Boise City-Nampa, ID MSA	616,561	1-2	2
¹ see http://www2.census.gov/econ/susb/data/msa_codes_2007_to_2011.txt ² Minimum monitoring requirements apply to the Metropolitan statistical area (MSA). CBSA includes both MSAs and micropolitan statistical areas. ³ Population based on latest available census figures.			

MSA population ^{1,2}	High concentration ²	Medium concentration ³	Low concentration ^{4 5}
>1 million	6-10	4-8	2-4
500K to 1 million	4-8	2-4	1-2
250K to 500K	3-4	1-2	0-1
100K to 250K	1-2	0-1	0
¹ Selection of urban areas and actual numbers of stations per area will be jointly determined by EPA and the State agency. ² High concentration areas are those for which ambient PM10 data show ambient concentrations exceeding the PM10 NAAQS by 20 percent or more. ³ Medium concentration areas are those for which ambient PM10 data show ambient concentrations exceeding 80 percent of the PM10 NAAQS. ⁴ Low concentration areas are those for which ambient PM10 data show ambient concentrations less than 80 percent of the PM10 NAAQS. ⁵ These minimum monitoring requirements apply in the absence of a design value.			

PART 58 APPENDIX D SITE EVALUATION FORM FOR SO₂

APPLICABLE SECTION	REQUIREMENT	CRITERIA MET?		
		YES	NO	N/A
4.4.1	State and, where appropriate, local agencies must operate a minimum number of required SO ₂ monitoring sites (based on PWEI calculation specified in 4.4.2 – use Table 1 and 2 below to determine minimum requirement for each CBSA)	X		
4.4.2(a)(1)	Is the monitor sited within the boundaries of the parent CBSA and is it one of the following site types: population exposure, highest concentration, source impacts, general background, or regional transport?	X		
4.4.3(a)	Has the EPA Regional Administrator required additional SO ₂ monitoring stations above the minimum number of monitors required in 4.4.2? If so, note location in comment field.	X*		
4.4.5(a)	Is your agency counting an existing SO ₂ monitor at an NCore site in a CBSA with a minimum monitoring requirement?	X		

Comments:
*DEQ is conducting source/highest concentration monitoring in Pocatello and Soda Springs.

CBSA Description ¹	CBSA population ²	total amount of SO ₂ in tons per year emitted within the CBSA (used 2011 NEI ⁴)	PWEI (population x total emissions ÷ 1,000,000)	Minimum required number of SO ₂ monitors in CBSA (see Table 2 below)	Present number of SO ₂ monitors in CBSA
Boise City, ID	616,561	2804.97	1729.44	0	1

¹see <http://www.census.gov/population/metro/data/def.html>
²Minimum monitoring requirements apply to the Core Based statistical area (CBSA). CBSA includes both metropolitan and micropolitan statistical areas.
³Population based on latest available census figures.
⁴see <http://www.epa.gov/ttn/chief/eiinformation.html>

PWEI (Population weighted Emission Index) Value	Require number of SO ₂ monitors
>= 1,000,000	3
>= 100,000 but < 1,000,000	2
>= 5,000 but < 100,000	1

PART 58 APPENDIX D SITE EVALUATION FORM FOR CARBON MONOXIDE (CO)

APPLICABLE SECTION	REQUIREMENT	OBSERVED	CRITERIA MET?		
			YES	NO	N/A
4.2.1(a)	One CO monitor is required to operate collocated with one required near-road NO ₂ monitor in CBSAs having a population of 1,000,000 or more persons. If a CBSA has more than one required near-road NO ₂ monitor, only one CO monitor is required to be collocated with a near-road NO ₂ monitor within that CBSA.		X*		
4.2.2(a)	Has the EPA Regional Administrator required additional CO monitoring stations above the minimum number of monitors required in 4.2.1? If so, note location in comment field.		X**		

Comments:

*As described in the network plan, DEQ is technically not required to operate a near road site presently, but DEQ chose to continue monitoring at the end of the pilot study to obtain an ongoing data record.

**DEQ has two additional monitors that are required. One is at DEQ's St. Lukes – Meridian, ID N-Core site, and the other one is at DEQ's Boise – Eastman CO maintenance area site.

MSA Description ¹	CBSA population ^{2,3}	Minimum required number of SLAMS CO sites	Present number of SLAMS CO sites in MSA
Boise City-Nampa, ID MSA	616,561	1 – Near Road* 1 – N-Core** 1 – Maintenance Area**	3

¹see http://www2.census.gov/econ/susb/data/msa_codes_2007_to_2011.txt

²Minimum monitoring requirements apply to the Core Based statistical area (CBSA). CBSA includes both metropolitan and micropolitan statistical areas.

³Population based on latest available census figures.

PART 58 APPENDIX D SITE EVALUATION FORM FOR NITROGEN DIOXIDE (NO₂)

APPLICABLE SECTION	REQUIREMENT	CRITERIA MET?		
		YES	NO	N/A
4.3.2(a)	Near-road NO ₂ Monitors: One microscale near-road NO ₂ monitoring station in each CBSA with a population of 500,000 or more persons.	X*		
4.3.2(a)	Near-road NO ₂ Monitors: An additional near-road NO ₂ monitoring station is required for any CBSA with a population of 2,500,000 persons, or in any CBSA with a population of 500,000 or more persons that has one or more roadway segments with 250,000 or greater AADT count.			X
4.3.2(b)	Near-road NO ₂ Monitors: Measurements at required near-road NO ₂ monitor sites utilizing chemiluminescence FRMs must include at a minimum: NO, NO ₂ , and NO _x	X*		
4.3.3(a)	Area-wide NO ₂ Monitoring: One monitoring station in each CBSA with a population of 1,000,000 or more persons to monitor a location of expected highest NO ₂ concentrations representing the neighborhood or larger spatial scales.			X

Comments:

*As described in the network plan, DEQ is technically not required to operate a near road site presently, but DEQ chose to continue monitoring at the end of the pilot study to obtain an ongoing data record.

CBSA Description ¹	CBSA population ^{2,3}	Required number of Near-road NO ₂ sites	Present number of Near-road NO ₂ sites	Required number of Area-wide NO ₂ sites	Present number of Area-wide NO ₂ sites
Boise City-Nampa, ID MSA	616,561	1*	1*	0	0
¹ see http://www2.census.gov/econ/subs/data/msa_codes_2007_to_2011.txt ² Minimum monitoring requirements apply to the Core Based statistical area (CBSA). CBSA includes both metropolitan and micropolitan statistical areas. ³ Population based on latest available census figures.					

PART 58 APPENDIX D SITE EVALUATION FORM FOR OZONE

APPLICABLE SECTION	REQUIREMENT	CRITERIA MET?		
		YES	NO	N/A
4.1(b)	At least one O ₃ site for each MSA, or CSA if multiple MSAs are involved, must be designed to record the maximum concentration (note location in comment field).	X*		
4.1(c)	The appropriate spatial scales for O ₃ sites are neighborhood, urban, and regional (note deviations in comment field).	X		
4.1(f)	Confirm that the monitoring agency consulted with EPA R10 when siting the maximum O ₃ concentration site.	X		
4.1(i)	O ₃ is being monitored at SLAMS monitoring sites during the “ozone season” as specified in Table D-3 of Appendix D to Part 58.	X		

Comments:

*DEQ’s White Pine Elementary site in Boise serves as the maximum concentration site.

MSA Description ^a	MSA population ^{1,2}	Minimum required number of SLAMS O ₃ sites (from Table D-2)	Present number of SLAMS O ₃ sites in CBSA
Boise City – Nampa, ID MSA	616,561	2	2

^asee http://www2.census.gov/econ/susb/data/msa_codes_2007_to_2011.txt

Table D-2 of Appendix D to Part 58 - SLAMS O₃ Monitoring Minimum Requirements

MSA population ^{1,2}	Most recent 3-year design value concentrations ≥85% of any O ₃ NAAQS ³	Most recent 3-year design value concentrations <85% of any O ₃ NAAQS ^{3,4}
>10 million	4	2
4-10 million	3	1
350,000-<4 million	2	1
50,000-<350,000 ⁵	1	0

¹Minimum monitoring requirements apply to the Metropolitan statistical area (MSA). CBSA includes both MSAs and micropolitan statistical areas.

²Population based on latest available census figures.

³The ozone (O₃) National Ambient Air Quality Standards (NAAQS) levels and forms are defined in 40 CFR part 50.

⁴These minimum monitoring requirements apply in the absence of a design value.

⁵Metropolitan statistical areas (MSA) must contain an urbanized area of 50,000 or more population.

**Table D-3 of Appendix D to Part 58—
Ozone Monitoring Season by State**

State	Begin month	End Month
Alaska	April	October
Idaho	May	September
Oregon	May	September
Washington	May	September

PART 58 APPENDIX E SITE EVALUATION FORM FOR CO

SITE NAME Eastman SITE ADDRESS 166 N. 9th Street, Boise ID 83702
 AQS ID 160010014 EVALUATION DATE 5/15/2015 EVALUATOR Leah Arnold - Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	For neighborhood or larger spatial scale sites the probe must be located 2-15 meters above ground level and must be at least 1 meter vertically or horizontally away from any supporting structure, walls, <i>etc.</i> , and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood scale avoid placing the monitor probe inlet near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site.	Eastman is a microscale site.			X
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the probe inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet (exception is street canyon or source-oriented sites where buildings and other structures are unavoidable).		X		
	(b) The probe inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the probe inlet must be at least 10 meters or further from the drip line of trees.			X*	
	(c) No trees should be between source and probe inlet for microscale sites.		X**		
6. SPACING FROM ROADWAYS	2. (b) Microscale CO monitor probes in downtown areas or urban street canyon locations shall be located a minimum distance of 2 meters and a maximum distance of 10 meters from the edge of the nearest traffic lane.			X***	
	2. (c) Microscale CO monitor inlet probes in downtown areas or urban street canyon locations shall be located at least 10 meters from an intersection and preferably at a midblock location.		X		
9. PROBE MATERIAL & RESIDENCE TIME	(a) Sampling train material must be FEP Teflon or borosilicate glass (e.g., Pyrex) for reactive gases.		X		
	(c) Sampling probes for reactive gas monitors at NCore must have a sample residence time less than 20 seconds.		X****		

Are there any changes that might compromise original siting criteria? If so, provide detail in comment section.

Other Comments:
 *Probe inlet is approximately 1 meter from tree branch. The City of Boise has worked with DEQ to keep the tree trimmed, but cutting the tree down is not favored.
 **Trees are on North and South sides of probe inlet and not the West side where the traffic (CO source) occurs.
 ***Probe inlet is located at approximately 0.5 meters horizontally from nearest traffic lane. DEQ used a lamp post to route, conceal, and protect the probe line in. This lamp post is positioned 0.5 meters from the nearest traffic lane.
 ****This site is not an N-Core site. Its sample residence time is longer than 20 seconds.

PART 58 APPENDIX E SITE EVALUATION FORM FOR CO					
SITE NAME <u>N-Core</u> SITE ADDRESS <u>Eagle Road & I-84, Meridian ID 83642</u>					
AQSD ID <u>160010010</u> EVALUATION DATE <u>5/15/2015</u> EVALUATOR <u>Ed Jolly - Idaho DEQ</u>					
APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	For neighborhood or larger spatial scale sites the probe must be located 2-15 meters above ground level and must be at least 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood scale avoid placing the monitor probe inlet near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the probe inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet (exception is street canyon or source-oriented sites where buildings and other structures are unavoidable).		X		
	(b) The probe inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the probe inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	2. (b) Microscale CO monitor probes in downtown areas or urban street canyon locations shall be located a minimum distance of 2 meters and a maximum distance of 10 meters from the edge of the nearest traffic lane.				X
	2. (c) Microscale CO monitor inlet probes in downtown areas or urban street canyon locations shall be located at least 10 meters from an intersection and preferably at a midblock location.				X
9. PROBE MATERIAL & RESIDENCE TIME	(a) Sampling train material must be FEP Teflon or borosilicate glass (e.g., Pyrex) for reactive gases.		X		
	(c) Sampling probes for reactive gas monitors at NCore must have a sample residence time less than 20 seconds.		X		
Are there any changes that might compromise original siting criteria? If so, provide detail in comment section. No.					
Other Comments:					

Roadway average daily traffic, vehicles per day	Minimum distance ¹ (meters)
≤10,000	10
15,000	25
20,000	45
30,000	80
40,000	115
50,000	135
≥60,000	150

¹ Distance from the edge of the nearest traffic lane. The distance for intermediate traffic counts should be interpolated from the table values based on the actual traffic count.

PART 58 APPENDIX E SITE EVALUATION FORM FOR CO

SITE NAME Near Roadway SITE ADDRESS 1311 East Central Drive, Meridian ID 83642
 AQS ID 160010023 EVALUATION DATE 5/15/2015 EVALUATOR Ed Jolly – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICAL PLACEMENT	For neighborhood or larger spatial scale sites the probe must be located 2-15 meters above ground level and must be at least 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood scale avoid placing the monitor probe inlet near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the probe inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet (exception is street canyon or source-oriented sites where buildings and other structures are unavoidable).		X		
	(b) The probe inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the probe inlet must be at least 10 meters or further from the drip line of trees.			X*	
	(c) No trees should be between source and probe inlet for microscale sites.		X		
6. SPACING FROM ROADWAYS	2. (b) Microscale CO monitor probes in downtown areas or urban street canyon locations shall be located a minimum distance of 2 meters and a maximum distance of 10 meters from the edge of the nearest traffic lane.				X
	2. (c) Microscale CO monitor inlet probes in downtown areas or urban street canyon locations shall be located at least 10 meters from an intersection and preferably at a midblock location.				X
9. PROBE MATERIAL & RESIDENCE TIME	(a) Sampling train material must be FEP Teflon or borosilicate glass (e.g., Pyrex) for reactive gases.		X		
	(c) Sampling probes for reactive gas monitors at NCore must have a sample residence time less than 20 seconds.		X		
Are there any changes that might compromise original siting criteria? If so, provide detail in comment section. No.					

Other Comments:

*Tree is 6.8 meters from inlet. Total height of tree is only approximately 0.5 meters above inlet.

Roadway average daily traffic, vehicles per day	Minimum distance ¹ (meters)
≤10,000	10
15,000	25
20,000	45
30,000	80
40,000	115
50,000	135
≥60,000	150

¹ Distance from the edge of the nearest traffic lane. The distance for intermediate traffic counts should be interpolated from the table values based on the actual traffic count.

PART 58 APPENDIX E SITE EVALUATION FORM FOR NO, NO_x, NO₂, and NO_y

SITE NAME N-Core SITE ADDRESS Eagle Road & I-84, Meridian ID 83642

AQS ID 160010010 EVALUATION DATE 5/15/2015

EVALUATOR Ed Jolly - Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	For neighborhood or larger spatial scale sites the probe must be located 2-15 meters above ground level and must be at least 1 meter vertically or horizontally away from any supporting structure, walls, <i>etc.</i> , and away from dusty or dirty areas. Microscale near-road NO ₂ monitoring sites are required to have sampler inlets between 2 and 7 meters above ground level. If located near the side of a building or wall, then locate the sampler probe on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood scale and larger avoid placing the monitor probe inlet near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the probe inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The probe inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential.		X		
	(d) For near-road NO ₂ monitoring stations, the monitor probe shall have an unobstructed air flow, where no obstacles exist at or above the height of the monitor probe, between the monitor probe and the outside nearest edge of the traffic lanes of the target road segment.				X
5. SPACING FROM TREES	(a) To reduce possible interference the probe inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	See spacing requirements table below		X		
9. PROBE MATERIAL & RESIDENCE TIME	(a) Sampling train material must be FEP Teflon or borosilicate glass (e.g., Pyrex).		X		
	(c) Sampling probes for reactive gas monitors at NCore and at NO ₂ sites must have a sample residence time less than 20 seconds.		X		
Are there any changes that might compromise original siting criteria? If so, provide detail in comment section. No.					
Other Comments:					

¹Distance from the edge of the nearest traffic lane. The distance for intermediate traffic counts should be interpolated from the table values based on the actual traffic count.

²Applicable for ozone monitors whose placement has not already been approved as of December 18, 2006.

Roadway average daily traffic, vehicles per day	Minimum distance ¹ (meters)	Minimum distance ^{1, 2} (meters)
≤1,000	10	10
10,000	10	20
15,000	20	30
20,000	30	40
40,000	50	60
70,000	100	100
≥110,000	250	250

PART 58 APPENDIX E SITE EVALUATION FORM FOR NO, NO_x, NO₂, and NO_y

SITE NAME Near Roadway SITE ADDRESS 1311 East Central Drive, Meridian ID 83642

AQS ID 160010023 EVALUATION DATE 5/15/2015

EVALUATOR Ed Jolly – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	For neighborhood or larger spatial scale sites the probe must be located 2-15 meters above ground level and must be at least 1 meter vertically or horizontally away from any supporting structure, walls, <i>etc.</i> , and away from dusty or dirty areas. Microscale near-road NO ₂ monitoring sites are required to have sampler inlets between 2 and 7 meters above ground level. If located near the side of a building or wall, then locate the sampler probe on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood scale and larger avoid placing the monitor probe inlet near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the probe inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The probe inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential.		X		
	(d) For near-road NO ₂ monitoring stations, the monitor probe shall have an unobstructed air flow, where no obstacles exist at or above the height of the monitor probe, between the monitor probe and the outside nearest edge of the traffic lanes of the target road segment.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the probe inlet must be at least 10 meters or further from the drip line of trees.			X*	
	(c) No trees should be between source and probe inlet for microscale sites.		X		
6. SPACING FROM ROADWAYS	See spacing requirements table below		X**		
9. PROBE MATERIAL & RESIDENCE TIME	(a) Sampling train material must be FEP Teflon or borosilicate glass (e.g., Pyrex).		X		
	(c) Sampling probes for reactive gas monitors at NCore and at NO ₂ sites must have a sample residence time less than 20 seconds.		X		
Are there any changes that might compromise original siting criteria? If so, provide detail in comment section. No.					
Other Comments: *Tree is 6.8 meters from inlet. Total height of tree is only approximately 0.5 meters above inlet. **Meets the near-roadway specific requirements per the near-roadway Technical Assistance Document.					

¹Distance from the edge of the nearest traffic lane. The distance for intermediate traffic counts should be interpolated from the table values based on the actual traffic count.

²Applicable for ozone monitors whose placement has not already been approved as of December 18, 2006.

Roadway average daily traffic, vehicles per day	Minimum distance ¹ (meters)	Minimum distance ^{1,2} (meters)
≤1,000	10	10
10,000	10	20
15,000	20	30
20,000	30	40
40,000	50	60
70,000	100	100
≥110,000	250	250

PART 58 APPENDIX E SITE EVALUATION FORM FOR O3

SITE NAME N-Core SITE ADDRESS Eagle Road & I-84, Meridian, ID 83642

AQS ID 160010010 EVALUATION DATE 5/15/2015 EVALUATOR Ed Jolly - Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood scale avoid placing the monitor probe inlet near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site.		X		
	(b) To minimize scavenging effects, the probe inlet must be away from furnace or incineration flues or other minor sources of SO ₂ or NO.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the probe inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The probe inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the probe inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.				X*
6. SPACING FROM ROADWAYS	See spacing requirements table below		X		
9. PROBE MATERIAL & RESIDENCE TIME	(a) Sampling train material must be FEP Teflon or borosilicate glass (e.g., Pyrex).		X		
	(c) Sampling probes for reactive gas monitors at NCore must have a sample residence time less than 20 seconds.		X		
Are there any changes that might compromise original siting criteria? If so, provide detail in comment section. No.					
Other Comments:					
*Not a microscale site.					

Roadway average daily traffic, vehicles per day	Minimum distance ¹ (meters)	Minimum distance ^{1,2} (meters)
≤1,000	10	10
10,000	10	20
15,000	20	30
20,000	30	40
40,000	50	60
70,000	100	100
≥110,000	250	250

¹Distance from the edge of the nearest traffic lane. The distance for intermediate traffic counts should be interpolated from the table values based on the actual traffic count.

²Applicable for ozone monitors whose placement has not already been approved as of December 18, 2006.

PART 58 APPENDIX E SITE EVALUATION FORM FOR O3

SITE NAME White Pine Elementary SITE ADDRESS 401 E. Linden St., Boise ID 83706
 AQS ID 160010017 EVALUATION DATE 5/15/2015 EVALUATOR Ed Jolly/Leah Arnold - Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood scale avoid placing the monitor probe inlet near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site.		X		
	(b) To minimize scavenging effects, the probe inlet must be away from furnace or incineration flues or other minor sources of SO ₂ or NO.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the probe inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The probe inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the probe inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.				X*
6. SPACING FROM ROADWAYS	See spacing requirements table below		X		
9. PROBE MATERIAL & RESIDENCE TIME	(a) Sampling train material must be FEP Teflon or borosilicate glass (e.g., Pyrex).		X		
	(c) Sampling probes for reactive gas monitors at NCore must have a sample residence time less than 20 seconds.		X		
Are there any changes that might compromise original siting criteria? If so, provide detail in comment section. No.					
Other Comments: *Not a microscale site.					

Roadway average daily traffic, vehicles per day	Minimum distance ¹ (meters)	Minimum distance ^{1,2} (meters)
≤1,000	10	10
10,000	10	20
15,000	20	30
20,000	30	40
40,000	50	60
70,000	100	100
≥110,000	250	250

¹Distance from the edge of the nearest traffic lane. The distance for intermediate traffic counts should be interpolated from the table values based on the actual traffic count.
²Applicable for ozone monitors whose placement has not already been approved as of December 18, 2006.

PART 58 APPENDIX E SITE EVALUATION FORM FOR SO2

SITE NAME N-Core SITE ADDRESS Eagle Road & I-84, Meridian ID 83642
 AQS ID 160010010 EVALUATION DATE 5/15/2015 EVALUATOR Ed Jolly – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level. 1 meter vertically or horizontally away from any supporting structure, walls, <i>etc.</i> , and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood scale avoid placing the monitor probe inlet near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the probe inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The probe inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the probe inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	There are no roadway spacing requirements for SO2.				X
9. PROBE MATERIAL & RESIDENCE TIME	(a) Sampling train material must be FEP Teflon or borosilicate glass (e.g., Pyrex).		X		
	(c) Sampling probes for reactive gas monitors at NCore must have a sample residence time less than 20 seconds.		X		
Are there any changes that might compromise original siting criteria? If so, provide detail in comment section. No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR SO2

SITE NAME Pocatello Sewage Treatment Plant SITE ADDRESS Batiste Chubbuck Rd., Pocatello ID 83204
 AQS ID 160050004 EVALUATION DATE 5/15/2015 EVALUATOR Marshall Magee – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood scale avoid placing the monitor probe inlet near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site.	Site is Middle Scale.			X
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the probe inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The probe inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the probe inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.		X		
6. SPACING FROM ROADWAYS	There are no roadway spacing requirements for SO2.				X
9. PROBE MATERIAL & RESIDENCE TIME	(a) Sampling train material must be FEP Teflon or borosilicate glass (e.g., Pyrex).		X		
	(c) Sampling probes for reactive gas monitors at NCore must have a sample residence time less than 20 seconds.		X		
Are there any changes that might compromise original siting criteria? If so, provide detail in comment section. No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR SO2

SITE NAME Soda Springs SITE ADDRESS 5-mile Road, Soda Springs ID 83276

AQS ID 160290031 EVALUATION DATE 5/15/2015 EVALUATOR Marshall Magee – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level. 1 meter vertically or horizontally away from any supporting structure, walls, <i>etc.</i> , and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood scale avoid placing the monitor probe inlet near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site.	Site is Middle-Micro Scale.			X
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the probe inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The probe inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the probe inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.		X		
6. SPACING FROM ROADWAYS	There are no roadway spacing requirements for SO2.				X
9. PROBE MATERIAL & RESIDENCE TIME	(a) Sampling train material must be FEP Teflon or borosilicate glass (e.g., Pyrex).		X		
	(c) Sampling probes for reactive gas monitors at NCore must have a sample residence time less than 20 seconds.		X		
Are there any changes that might compromise original siting criteria? If so, provide detail in comment section. No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Athol SITE ADDRESS NE corner of Pastime St. and Grove Ave., Athol ID 83801

AQS ID N/A EVALUATION DATE 5/21/2015

EVALUATOR Shawn Sweetapple – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.			X*	
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					

Other Comments:

* A pump house is located 2.5 meters away from the monitor. The pump house height is 2.8 meters above the height of the inlet. This monitor (nephelometer) is operated seasonally and is not a SLAMS site. The predominant wind direction during the season of highest pollutant concentration is from the South and not impeded by the pump house.

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Boise Fire Station SITE ADDRESS 16th and Front Street, Boise ID 83702

AQS ID 160010009 EVALUATION DATE 5/15/2015

EVALUATOR Leah Arnold - Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Cottonwood SITE ADDRESS BLM Field Office – 1 Butte Dr., Cottonwood ID 83522

AQS ID N/A EVALUATION DATE 5/18/2015

EVALUATOR Zac Bishop – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.			X*	
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.			X**	
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
<p>Other Comments:</p> <p>* A tree is located 6 meters away from the monitor. The tree height is 7 meters above the height of the inlet. This monitor (nephelometer) is operated seasonally and is not a SLAMS site. The predominant wind direction during the season of highest pollutant concentration is not impeded by the tree.</p> <p>**The monitor is approximately 6 meters from the drip line of a tree.</p>					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Franklin SITE ADDRESS East 4800 South Road, Franklin ID 83237

AQS ID 160410001 EVALUATION DATE 5/15/2015

EVALUATOR Marshall Magee – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Garden Valley SITE ADDRESS 946 Banks Lowman Rd., Garden Valley ID 83622

AQS ID 160150002 EVALUATION DATE 5/15/2015

EVALUATOR Leah Arnold – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Garwood SITE ADDRESS 17506 N. Ramsey Rd., Rathdrum ID 83858

AQS ID N/A EVALUATION DATE 5/21/2015

EVALUATOR Shawn Sweetapple – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.			X*	
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					

Other Comments:

*The monitor is located on school grounds as a way to assess pollutants at a site with sensitive populations. This monitor (nephelometer) is operated seasonally and is not a SLAMS site. The predominant wind direction during the season of highest pollutant concentration is from the West and not impeded by the school building.

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Grangeville SITE ADDRESS USFS Compound – Grangeville ID 83530

AQS ID 160490002 EVALUATION DATE 5/18/2015

EVALUATOR Zac Bishop – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Idaho City SITE ADDRESS 3851 Hwy 21, Idaho City ID 83631

AQS ID 160150001 EVALUATION DATE 5/15/2015

EVALUATOR Leah Arnold – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Idaho Falls SITE ADDRESS Hickory and Sycamore Streets, Idaho Falls ID 83402

AQS ID 160190011 EVALUATION DATE 5/18/2015

EVALUATOR Ryan Rossi – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Kendrick SITE ADDRESS Kendrick Pump Station, Kendrick ID 83537

AQS ID N/A EVALUATION DATE 5/18/2015

EVALUATOR Zac Bishop – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.			X*	
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments: *The monitor is approximately 8 meters from the drip line of a tree.					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Ketchum SITE ADDRESS 111 West 8th Street, Ketchum ID 83340

AQS ID 160130004 EVALUATION DATE 5/11/2015

EVALUATOR Drew Jones – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Lancaster SITE ADDRESS West Lancaster Rd., Hayden, ID 83835

AQS ID 160550003 EVALUATION DATE 5/21/2015

EVALUATOR Shawn Sweetapple – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Lewiston SITE ADDRESS 1200 29th Street, Lewiston ID 83501

AQS ID 160690012 EVALUATION DATE 5/18/2015

EVALUATOR Zac Bishop – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME McCall SITE ADDRESS 500 N. Mission Street, McCall ID 83638

AQS ID 160850002 EVALUATION DATE 5/15/2015

EVALUATOR Leah Arnold - Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.			X*	
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments: *Small tree is located at 8.7 meters away from monitor.					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Moscow SITE ADDRESS 1025 Plant Sciences Rd., Moscow ID 83843

AQS ID 160570005 EVALUATION DATE 5/18/2015

EVALUATOR Zac Bishop – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Mt. Hall SITE ADDRESS 1275 Idaho 1, Bonners Ferry ID 83805

AQS ID N/A EVALUATION DATE 5/21/2015

EVALUATOR Shawn Sweetapple – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Nampa SITE ADDRESS Nampa Fire Station – 923 1st Street South, Nampa ID 83651

AQS ID 160270002 EVALUATION DATE 5/15/2015

EVALUATOR Leah Arnold – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME N-Core SITE ADDRESS Eagle Road & I-84, Meridian ID 83642

AQS ID 160010010 EVALUATION DATE 5/15/2015

EVALUATOR Ed Jolly - Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Paul SITE ADDRESS 201 N. 1st Street West, Paul ID 83347

AQS ID N/A EVALUATION DATE 5/11/2015

EVALUATOR Drew Jones – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.			X*	
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.			X**	
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? See below.					
Other Comments: *Tree stands 5.1 meters taller than probe inlet. Tree is only located 5.2 meters away from probe inlet. **Tree is located 5.2 meters away from probe inlet. Higher branches overhang probe inlet. DEQ will contact the school where the monitor is located to try to get approval for tree to be trimmed.					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Pinehurst SITE ADDRESS 106 Church Street, Pinehurst ID 83850

AQS ID 160790017 EVALUATION DATE 5/21/2015

EVALUATOR Shawn Sweetapple – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Pocatello SITE ADDRESS Corner of Garrett and Gould Streets, Pocatello ID 83204

AQS ID 160050015 EVALUATION DATE 5/15/2015

EVALUATOR Marshall Magee – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Porthill SITE ADDRESS Tavern Farm Rd., Porthill ID 83853

AQS ID N/A EVALUATION DATE 5/21/2015

EVALUATOR Shawn Sweetapple - Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sties. 1 meter vertically or horizontally away from any supporting structure, walls, <i>etc.</i> , and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Potlatch SITE ADDRESS 510 Elm Street, Potlatch ID 83855

AQS ID N/A EVALUATION DATE 5/18/2015

EVALUATOR Zac Bishop – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Rexburg SITE ADDRESS Madison Middle School – 575 W. 7th Street, Rexburg ID 83440

AQS ID N/A EVALUATION DATE 5/18/2015

EVALUATOR Ryan Rossi – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Salmon SITE ADDRESS N. Charles Street, Salmon ID 83467

AQS ID 160590004 EVALUATION DATE 5/18/2015

EVALUATOR Ryan Rossi – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Sandpoint SITE ADDRESS U of I Research Center – 2105 N. Boyer Ave., Sandpoint ID 83864

AQS ID 160170003 EVALUATION DATE 5/21/2015

EVALUATOR Shawn Sweetapple – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Soda Springs SITE ADDRESS Caribou Hospital – 300 S. 3rd Street West, Soda Springs ID 83276

AQS ID N/A EVALUATION DATE 5/15/2015

EVALUATOR Marshall Magee – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME St. Maries SITE ADDRESS USFS Building - St. Maries ID, 83666

AQS ID 160090010 EVALUATION DATE 5/21/2015

EVALUATOR Shawn Sweetapple - Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Twin Falls SITE ADDRESS 650 W. Addison, Twin Falls ID 83301

AQS ID 160830007 EVALUATION DATE 5/11/2015

EVALUATOR Drew Jones – Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					

PART 58 APPENDIX E SITE EVALUATION FORM FOR PM2.5, PM10, PM10-2.5, and Pb

SITE NAME Weiser SITE ADDRESS 690 W. Indianhead Rd., Weiser ID 83672

AQS ID N/A EVALUATION DATE 5/15/2015

EVALUATOR Leah Arnold - Idaho DEQ

APPLICABLE SECTION	REQUIREMENT	COMMENTS	CRITERIA MET?		
			YES	NO	N/A
2. HORIZONTAL AND VERTICLE PLACEMENT	2-15 meters above ground level (AGL) for neighborhood or larger spatial scale, 2-7 meters for microscale spatial scale sites and middle spatial scale PM _{10-2.5} sites. 1 meter vertically or horizontally away from any supporting structure, walls, etc., and away from dusty or dirty areas. If located near the side of a building or wall, then locate on the windward side relative to the prevailing wind direction during the season of highest concentration potential.		X		
3. SPACING FROM MINOR SOURCES	(a) For neighborhood or larger spatial scales avoid placing the monitor near local, minor sources. The source plume should not be allowed to inappropriately impact the air quality data collected at a site. Particulate matter sites should not be located in an unpaved area unless there is vegetative ground cover year round.		X		
4. SPACING FROM OBSTRUCTIONS	(a) To avoid scavenging, the inlet must have unrestricted airflow and be located away from obstacles. The separation distance must be at least twice the height that the obstacle protrudes above the probe inlet.		X		
	(b) The inlet must have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential. For particle sampling, a minimum of 2 meters of separation from walls, parapets, and structures is required for rooftop site placement.		X		
5. SPACING FROM TREES	(a) To reduce possible interference the inlet must be at least 10 meters or further from the drip line of trees.		X		
	(c) No trees should be between source and probe inlet for microscale sites.	Not a microscale site			X
6. SPACING FROM ROADWAYS	Spacing from roadways is dependent on the spatial scale and ADT count. See section 6.3(b) and figure E-1 for specific requirements.		X		
Are there any changes that might compromise original siting criteria? No.					
Other Comments:					