

Note: This is a reference cited in AP 42, *Compilation of Air Pollutant Emission Factors, Volume I Stationary Point and Area Sources*. AP42 is located on the EPA web site at [www.epa.gov/ttn/chief/ap42/](http://www.epa.gov/ttn/chief/ap42/)

The file name refers to the reference number, the AP42 chapter and section. The file name "ref02\_c01s02.pdf" would mean the reference is from AP42 chapter 1 section 2. The reference may be from a previous version of the section and no longer cited. The primary source should always be checked.

AP42 Section:	11.27
Reference:	3
Title:	<i>Source Sampling Report For The Feldspar Corporation: Spruce Pine, NC, Environmental Testing Inc., Charlotte, NC, May 1979.</i>

RECEIVED JUL  
AP-42 Section 11.27  
Reference 3  
Report Sect. 4  
Reference 1

RECEIVED JUN 14 1977 A-82-39  
II-A-62

RECEIVED  
Water Quality Division  
JUN 11 1979  
Western Regional Office  
Asheville, North Carolina

SOURCE SAMPLING REPORT  
for  
FELDSPAR CORPORATION  
Spruce Pine, North Carolina

Performed by:

ENVIRONMENTAL TESTING, INC.  
Charlotte, North Carolina  
5178

*James S. McCormack*  
James S. McCormack  
NORTH CAROLINA PROFESSIONAL SEAL  
5/29/78

## TABLE OF CONTENTS


INTRODUCTION	1
SUMMARY OF RESULTS	3
PROCESS DESCRIPTION AND OPERATION	5
LOCATION OF SAMPLING POINTS	6
SAMPLING AND ANALYTICAL PROCEDURES	8
APPENDICIES	9
A. Particulate Results and Calculations	
B. Field Data	
C. Test Participants	
D. Sampling and Analytical Procedures	
E. Calibration Data	

## INTRODUCTION

Source sampling was performed on a feldspar dryer for Feldspar Corporation, Spruce Pine, North Carolina, to determine particulate emissions. Three particulate sampling runs were made on May 16, 1979. Sampling locations are shown on Figure 1.

The measurements of stack gas flow rate, gas composition and particulate emissions were made according to the recommendations of the U. S. Environmental Protection Agency and the North Carolina Department of Natural Resources and Community Development (DNRCD). Mr. W. L. Anderson and Ms. Deborah Hale, DNRCD, were present as observers.

The following sections of the report treat the summary of results, a description of the process and its operation, the location of the sampling points and the sampling and analytical procedures used.

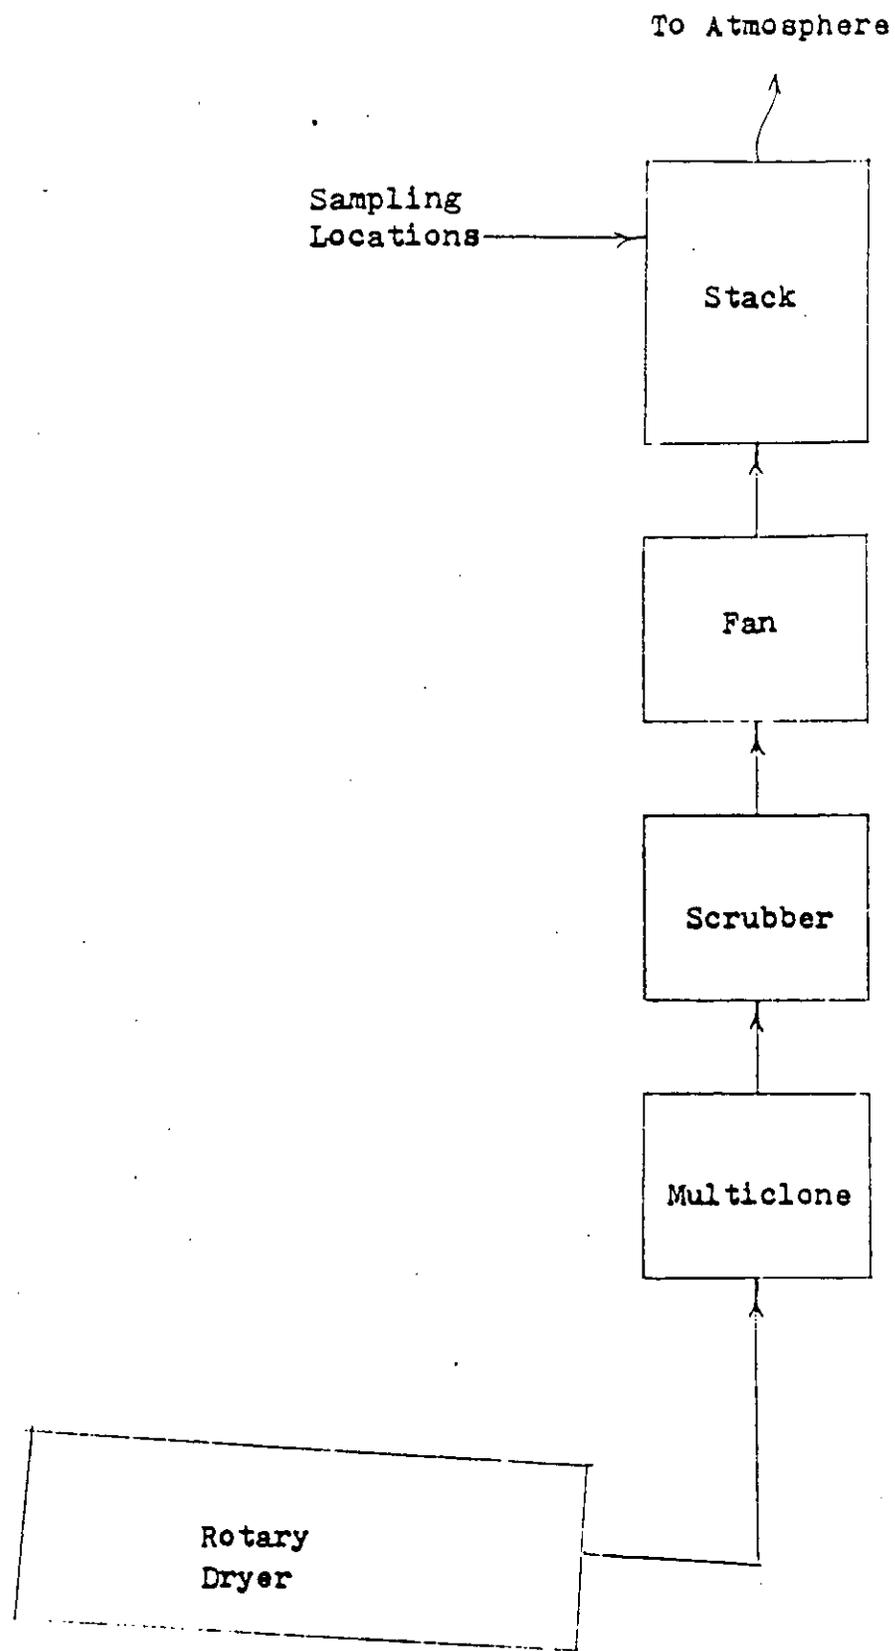

SAMPLING LOCATION  
Figure 1

## SUMMARY OF RESULTS

Table 1 presents a summary of results from the particulate source sampling. For the three isokinetic runs the mean particulate emission rate was 0.0167 grains per dry standard cubic foot and 1.50 pounds per hour. Process weight was determined from the average of production records as 10 tons (20,000 pounds) per hour.

Based on North Carolina Administrative Code, Title 15, Chapter 2, Subchapter 2D, Section .0509, Particulates from Mica or Feldspar Processing Plants, the allowable emission rate is 19.0 pounds per hour. Consequently, Feldspar Corporation Plant No. 2 feldspar dryer is in compliance with the regulation.

TABLE 1

## SUMMARY OF RESULTS, PARTICULATE TESTING

Run Number	1	2	3
Date	5/16/79	5/16/79	5/16/79
% Isokinetic	97.9	97.2	97.9
Stack Gas Flow Rate, SCFM * Dry	10,630	10,385	10,416
Stack Gas Flow Rate, ACFM	12,689	12,481	12,597
Volume of Gas Sampled, SCF * Dry	40.61	39.39	39.80
Process Weight, lbs/hr	20,000	20,000	20,000
Particulates:			
Catch-mgrams	40.3	35.9	53.6
Concentration-grains/ SCF * Dry	0.0153	0.0140	0.0207
Emission Rate, lbs/hr	1.39	1.25	1.85

\* 68°F, 29.92 in Hg

• • Front Half only


## PROCESS DESCRIPTION AND OPERATION

The rotary dryer at Feldspar Corporation, Spruce Pine, North Carolina, was used to dry processed feldspar. The dryer was fired with 50 gallons per hour of No. 2 fuel oil. Exhaust gases from the dryer passed through a multiclone, a scrubber, a fan and out the stack to the atmosphere. No unusual conditions were noted during sampling.

## LOCATION OF SAMPLING POINTS


The dimensions of the stack and the location of the sampling ports are shown in Figure 2. The stack was divided into 20 equal areas. The ports were labelled A through E. Each point was sampled for 3 minutes which yielded a total sampling time of 60 minutes. The number of sampling points was determined by the distance of the ports from disturbances in the gas flow per Method 1, Federal Register, Vol. 42, No. 160, 18 August 1977.

$$\frac{2(20)(18)}{20+18} = 18.9''$$

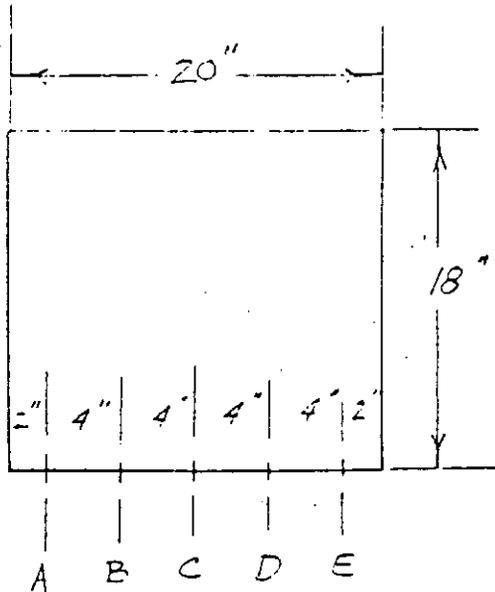

under 24",  $\frac{22}{55}$

1.26 Dia.

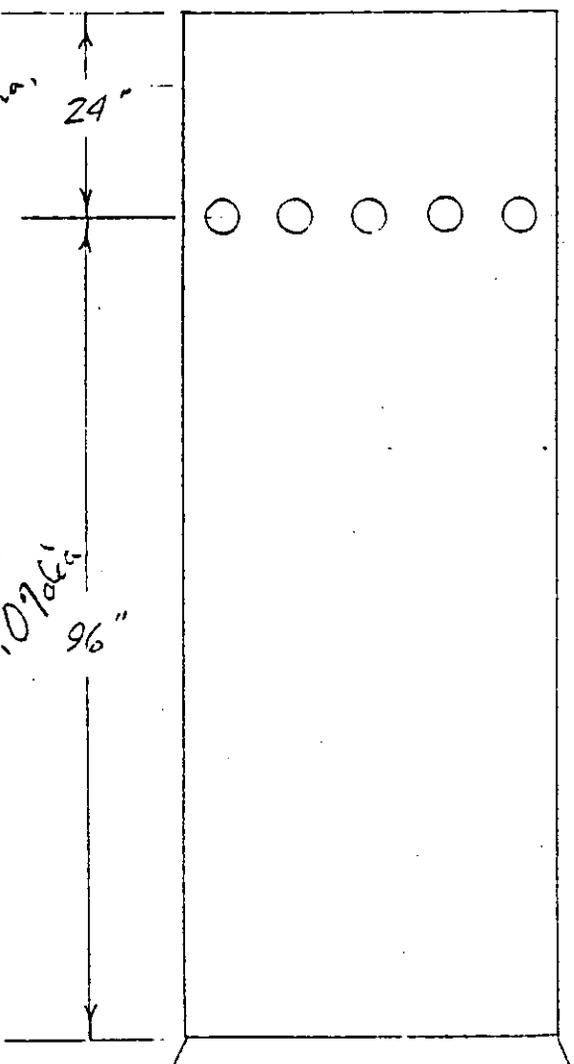

20 points  
WCCF

(2.5)  
5.07 Dia  
96"

SAMPLING PORTS AND POINTS

Figure 2

## SAMPLING AND ANALYTICAL PROCEDURES

All sampling and analytical procedures were those specified by the U. S. Environmental Protection Agency and the N. C. Department of Natural Resources and Community Development. Complete details are found in Appendix D, which is a copy of the Federal Register, Vol. 42, No. 160, 18 August 1977.

Sample point locations and velocity measurements were made by Methods 1 and 2. Gas composition was determined by Fyrite on Run 1 and by integrated bag samples on Runs 2 and 3 with an Orsat analyzer. Method 5 was used for particulate determination.

APPENDICIES

SUMMARY OF PARTICULATE RESULTS

- 1 FELDSPAR CORPORATION PLT. NO. 1
- 2 FELDSPAR CORPORATION PLT. NO. 2
- 3 FELDSPAR CORPORATION PLT. NO. 2

RUN NUMBER		1	2	3
TEST DATE		5/16/79	5/16/79	5/16/79
DN	SAMPLE NOZZLE DIA., IN	.173	.173	.173
TT	NET TIME OF TEST, MIN	60.0	60.0	60.0
PB	BAROMETRIC PRESSURE, IN	27.84	27.84	27.84
PM	AVERAGE ORIFICE PRESSURE DROP, IN H2O	1.640	1.549	1.600
VM	VOLUME OF DRY GAS SAMPLED CU FT AT METER CONDITIONS	45.090	44.080	44.520
TM	AVERAGE GAS METER TEMP DEGREES	87.6	91.8	91.7
VMSTD	VOLUME OF DRY GAS SAMPLED AT STANDARD CONDITIONS*, SCF	40.611	39.388	39.797
VW	TOTAL H2O COLLECTED IN IMPINGERS • SILICA GEL, ML	46.20	45.30	48.80
VMV	VOLUME OF WATER VAPOR AT STANDARD CONDITIONS*, SCF	2.175	2.132	2.297
PMV	PERCENT MOISTURE BY VOL	5.1	5.1	5.5
MD	MOLE FRACTION DRY GAS	.949	.949	.945
PCO2	PERCENT CO2 BY VOL., DRY	.60	1.30	1.55
PO2	PERCENT O2 BY VOL., DRY	18.13	18.25	18.00
PCO	PERCENT CO BY VOL., DRY	.00	.00	.00
PN2	PERCENT N2 BY VOL., DRY	81.27	80.45	80.45
MWD	MOLECULAR WT-DRY STK GAS	28.894	29.011	29.040
MW	MOLECULAR WT-STK GAS	28.340	28.446	28.438
CP	PITOT TUBE CCEFFICIENT	.84	.84	.84
DPS	AVERAGE VELOCITY HEAD OF STACK GAS, IN H2O	1.3970	1.3724	1.3830
TS	AVERAGE STACK TEMPERATURE	95.2	98.6	100.3

PS	STACK PRESSURE, ABSOLUTE	27.779	27.779	27.779
VS	AV STK GAS VELOCITY, FPM	5,054.85	4,972.00	5,018.50
AS	STACK AREA, IN SQRD	360.0	360.0	360.0
QS	STK FLOW RATE, DRY, STD COND	10,630	10,385	10,416
QSW	STK FLOW RATE, WET, STD COND	11,199	10,948	11,017
QA	ACTUAL STK FLOW RATE	12,689	12,481	12,597
PERI	PERCENT ISOKINETIC	97.9	97.2	97.9
FMF	PARTICULATE, MG, FRONT	40.3	35.9	53.6
CAN	PARTICULATE, GR/DSCF PARTIAL	.0153	.0140	.0207
CAM	PARTICULATE, GR/WSCF PARTIAL	.0161	.0148	.0219
CAT	PARTICULATE, GR/ACF PARTIAL	.0128	.0117	.0172
CAW	PARTICULATE, LB/HR PARTIAL	1.39	1.25	1.85
FNP	NET SAMPLING POINTS	20	20	20
RW	PROCESS WEIGHT, LB/HR	20,000	20,000	20,000

\*68 DEG F. 29.92 IN HG

PARTICULATE CALCULATIONS TEST NO. 3

F E L D S P A R C O R P O R A T I O N P L T . N O . 1

VOLUME OF DRY GAS SAMPLED AT STD. CONDITIONS

$$VMSTD = \frac{17.64 * VM * (PB + PM/13.6)}{TM + 460.} = 39.7971 \text{ DSCF}$$

VOLUME OF WATER VAPOR AT STD. CONDITIONS

$$VMV = .04707 * VW = 2.30 \text{ SCF}$$

PERCENT MOISTURE IN STACK GAS

$$PMV = \frac{100 * VMV}{VMSTD + VMV} = 5.46 \text{ PERCENT}$$

MOLE FRACTION OF DRY STACK GAS

$$MD = \frac{100 - PMV}{100} = .945$$

AVERAGE MOLECULAR WEIGHT OF DRY STACK GAS

$$MWD = .44 * PCO2 + .32 * PO2 + .28 * (PN2 + PCO) = 29.04$$

MOLECULAR WEIGHT OF STACK GAS

$$MW = MWD * MD + 18 * (1 - MD) = 28.44$$

STACK GAS VELOCITY AT STACK CONDITIONS

$$VS = 5129.4 * CP * DPS * \text{SQRT}(TS + 460) / (PS * MW) = 5,018.5 \text{ FP}$$

STACK GAS VOLUMETRIC FLOW AT STD. CONDITIONS, DRY

$$QS = \frac{.123 * VS * AS * PS * MD}{TS + 460} = 10,416 \text{ DSCFM}$$

STACK GAS VOLUMETRIC FLOW AT STACK CONDITIONS

$$CA = \frac{QS * (TS + 460)}{17.64 * PS * MD} = 12,597 \text{ ACFM}$$

PERCENT ISCKINETIC

$$\text{PERI} = \frac{1039 * (\text{TS} + 460) * \text{VMSTD}}{\text{VS} * \text{TT} * \text{PS} * \text{MD} * \text{DN} * \text{UN}} = 97.9 \text{ PERCENT}$$

PARTICULATE LOADING -- PROBE, CYCLONE, FILTER  
(AT STANDARD CONDITIONS)

$$\text{CAN} = .0154 * \text{FMF/VMSTD} = .021 \text{ GR/USCF}$$

PARTICULATE LOADING -- PROBE, CYCLONE, FILTER  
(AT STACK CONDITIONS)

$$\text{CAT} = \frac{17.64 * \text{CAN} * \text{PS} * \text{MD}}{\text{TS} + 460} = .0172 \text{ GR/ACF}$$

PARTICULATE LB/HR -- PROBE, CYCLONE, FILTER  
(AT STACK CONDITIONS)

$$\text{CAW} = .00857 * \text{CAN} * \text{QS} = 1.85 \text{ LB/HR}$$



cb = 9  
wb = 80

Methanol  
Eddy Sensor  
19 ppg

1.7  
2.3  
1.45  
2.2

10 lbs/ky  
W.L. Anderson  
Debbie Hale  
50 gal/ky #2 fuel oil

PARTICULATE FIELD DATA

Plant Feldspar Pit #2

Run No. 1

Location STK

Date 5/16/79

Operator JDM

Sample Box No. 1

Meter Box No. RAC #1

Meter  $\Delta H_1$  1.24

C Factor 98

Ambient Temp of 68°F

Bar. Press. in. Hg. 29.84

Assumed Moisture % 14%

Heater Box Setting, of 250

Probe Tip Dia., in. .173


Probe Length 4'

Probe Heater Setting 70%

Average  $\Delta p$  2.2

Average  $\Delta H$  1.23

VERY IMPORTANT - FILL IN ALL BLANKS  
Read and record at the start of each test point.



REMARKS:  
A B C D E @ 15"  
Leak Check @ 15 in Hg: .015, .004  
Static Pres., in H<sub>2</sub>O: -.83  
Start: 7:11  
Finish: 10:30  
Filter # 10

Point	Clock Time	Dry Gas Meter, Cu.ft.	Pilot Manometer ( $\Delta p$ ) In. H <sub>2</sub> O	Orifice Manometer ( $\Delta H$ ) In. H <sub>2</sub> O		Dry Gas Temp. or		Pump Vacuum In. Hg Gauge	Box Temp. of	Impinger Temp. of	Stack Temp. of	% CO <sub>2</sub>
				Desired	Actual	Inlet	Outlet					
2A	0	134.23	1.6	1.35	1.35	70	80	5.0	229	60	98	0.5
2	3	136.87	1.75	1.45	1.45	78	70	5.0	231	62	96	
2	6	137.95	1.85	1.55	1.55	82	72	5.0	235	60	96	
2	9	141.10	1.7	1.4	1.4	86	74	5.0	240	58	96	
2B	12	143.20	1.65	1.35	1.35	82	76	5.0	244	60	96	
2	3	145.25	1.8	1.5	1.5	86	76	6.0	248	58	96	
2	6	147.29	2.2	1.73	1.73	90	78	6.0	248	56	94	
2	9	147.81	2.2	1.73	1.73	92	78	6.0	248	54	94	
2	12	152.13	1.6	1.45	1.45	92	80	5.0	248	52	95	1.0
2	3	154.20	1.9	1.6	1.6	92	80	6.0	248	50	97	
2	6	156.40	2.25	1.85	1.85	92	82	7.0	249	48	95	
2	9	158.77	2.3	1.90	1.90	92	82	7.0	249	46	97	0.5
2B	12	161.15	1.65	1.4	1.4	100	84	5.5	249	44	97	
2	3	162.38	2.4	2.0	2.0	102	84	7.0	249	46	96	0.5
2	6	165.50	2.5	2.1	2.1	104	86	7.5	249	46	96	
2	9	168.20	2.55	2.1	2.1	104	86	7.5	249	46	96	
2B	12	172.43	1.4	1.15	1.15	104	84	4.5	249	47	96	
2	3	175.11	1.9	1.5	1.5	104	84	4.5	249	47	96	0.5
2	6	177.47	2.1	1.7	1.7	108	87	5.0	249	48	97	

70%

18.0

18.0

18.0

12.5



237 ml

**PARTICULATE FIELD DATA**

Plant Faldsper No 2 Run No. 2 Ambient Temp of 74

Location SAK Bar. Press. in. Hg. 29.84

Date 5/16/77 Assumed Moisture % 14%

Operator JSM Heater Box Setting, of 250

Sample Box No. 2 Probe Tip Dia., in. .173

Meter Box No. RAC #1 Probe Length 4'

Meter AH<sub>y</sub> 1.84 Probe Heater Setting 7070

C Factor .88 Average Ap 2.2

Average AH 1.83



REMARKS: ABOVE

@ 15" @ 8.11

Leak Check @ 15 in Hg: .020, .007

Static Pres., in H<sub>2</sub>O: 1.50

Finish: 1258

Filter # #13

Point	Clock Time	Dry Gas Meter, Cu. Ft.	Pitot Manometer (Ap) In. H <sub>2</sub> O	Orifice Manometer (AH) In. H <sub>2</sub> O		Dry Gas Temp. of		Pump Vacuum In. Hg Gauge	Box Temp. of	Impinger Temp. of	Stack Temp. of	% CO <sub>2</sub>
				Desired	Actual	Inlet	Outlet					
A 1	0	180.90	1.2	.98	.98	78	78	4.0	235	58	96	
2	3	182.68	1.75	1.45	1.45	84	80	3.5	228	56	97	
3	6	184.80	2.0	1.65	1.65	90	80	4.0	230	54	98	
4	9	187.08	2.1	1.75	1.75	96	82	4.0	239	51	100	
A 1	5/12	189.41	1.4	1.15	1.15	94	82	3.0	229	49	102	
2	3	191.37	1.8	1.45	1.45	96	84	3.5	230	47	101	
3	6	193.77	2.05	1.7	1.7	100	84	4.0	235	46	101	
4	9	196.11	2.2	2.0	2.0	102	86	4.5	237	46	102	
A 1	5/12	197.47	1.5	1.2	1.2	100	86	3.0	231	46	101	1.0
2	3	200.47	1.9	1.5	1.5	100	88	3.5	224	47	97	
3	6	202.78	2.4	2.0	2.0	104	87	4.5	227	45	97	
4	9	204.78	2.7	2.0	2.0	104	87	4.5	239	46	97	
A 1	5/12	207.15	1.0	1.05	1.05	100	88	1.5	202	47	97	
2	3	209.41	1.2	1.0	1.0	102	88	1.5	205	47	97	
3	6	211.49	2.05	1.75	1.75	102	88	4.0	205	47	97	
4	9	213.44	2.15	1.75	1.75	102	88	4.5	205	47	97	
A 1	5/12	215.25	1.6	1.3	1.3	100	88	3.5	204	47	97	
2	3	218.45	1.65	1.55	1.55	100	90	4.0	203	49	100	
3	6	220.69	1.95	1.6	1.6	100	90	4.10	201	49	101	



Vx. 8328 = AH 237 ml

PARTICULATE FIELD DATA

Plant Feldspar No 2 Run No. 3 Ambient Temp of 78

Location SHK Bar. Press. in. Hg. 27.84

Date 5/16/79 Assumed Moisture % 14%

Operator JSM Heater Box Setting, of 250


Sample Box No. 3 Probe Tip Dia., in. 4'

Meter Box No. RAC #1 Probe Length 70%

Meter ΔH<sub>y</sub> 1.84 Probe Heater Setting 2.2

C Factor .98 Average Δp 1.83

Leak Check @ 15 in Hg: .020, .006  
 Static Pres., in H<sub>2</sub>O: -.23  
 Start: 1420 Finish: 1531  
 Filter # 12

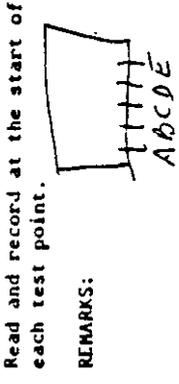

Read and record at the start of each test point.

REMARKS:

Point	Clock Time	Dry Gas Meter, Cu.ft.	Pitot Manometer (dp) in. H <sub>2</sub> O	Orifice Manometer (ΔH) in. H <sub>2</sub> O		Dry Gas Temp. °F		Pump Vacuum in. Hg Gauge	Box Temp. °F	Impinger Temp. °F	Stack Temp. °F	% CO <sub>2</sub>
				Desired	Actual	Inlet	Outlet					
E 1	0	226.83	1.6	1.3	1.3	80	80	3.5	87	58	99	
2	3	228.80	1.8	1.5	1.5	85	82	4.0	242	56	100	
3	6	230.99	2.0	1.65	1.65	88	82	4.5	237	54	100	
4	9	233.28	1.8	1.5	1.5	92	82	4.0	234	53	98	
D 1	0/12	235.47	2.1	1.75	1.75	92	82	4.0	236	50	97	
2	3	237.80	1.8	1.5	1.5	94	84	4.0	232	49	97	
3	6	239.99	2.1	1.75	1.75	96	84	4.5	229	47	98	
4	9	242.37	2.1	1.75	1.75	98	84	4.5	227	46	99	
C 1	12/0	244.79	1.0	1.3	1.3	98	84	3.5	232	46	99	
2	3	246.72	1.9	1.6	1.66	100	86	4.0	234	47	100	
3	6	248.92	2.3	1.85	1.85	102	86	4.5	235	48	100	
4	9	251.30	2.3	1.9	1.9	104	88	5.0	241	47	100	
B 1	0/12	253.78	1.5	1.25	1.25	102	88	3.5	236	48	101	
2	3	255.82	2.3	1.9	1.9	102	88	4.0	239	48	102	
3	6	257.83	2.4	2.0	2.0	102	88	5.5	234	49	103	
4	9	260.49	2.4	2.0	2.0	105	88	5.5	231	49	98	
A 1	12/0	262.47	1.3	1.1	1.1	103	90	3.5	233	50	103	
2	3	264.30	1.6	1.3	1.3	103	90	4.0	232	51	105	
3	6	266.97	1.8	1.5	1.5	104	90	4.5	226	53	103	



ORSAT ANALYSIS AND DRY MOLECULAR WEIGHT DETERMINATION

COMMENTS:

PLANT Feldspar Corp Pkt # 2

DATE 5/16/79

SAMPLING TIME (24-hr CLOCK) 0911-1030

SAMPLING LOCATION Stk

SAMPLE TYPE (BAG, INTEGRATED, CONTINUOUS) Grab

ANALYTICAL METHOD Fyrite

AMBIENT TEMPERATURE 68°F

OPERATOR JSM

*Run 1*

GAS	1		2		3		AVERAGE NET VOLUME	MULTIPLIER	MOLECULAR WEIGHT OF STACK GAS-DRY BASIS M <sub>d</sub> lb/lb-mole
	ACTUAL READING	NET	ACTUAL READING	NET	ACTUAL READING	NET			
CO <sub>2</sub>							0.600	144/100	1.264
O <sub>2</sub> (NET IS ACTUAL O <sub>2</sub> READING MINUS ACTUAL CO <sub>2</sub> )							18.125	32/100	5.8
CO (NET IS ACTUAL CO READING MINUS ACTUAL O <sub>2</sub> )							0.060	28/100	
N <sub>2</sub> (NET IS 100 MINUS ACTUAL CO)							21.275	28/100	22.151
TOTAL									28.82

*See Data Sheet*

ORSAT ANALYSIS AND DRY MOLECULAR WEIGHT DETERMINATION

COMMENTS:

PLANT Feldspar Corp Pkt #1

DATE 5/16/17

SAMPLING TIME (24-hr CLOCK) 1150-1258

SAMPLING LOCATION 57K

SAMPLE TYPE (BAG, INTEGRATED, CONTINUOUS)

ANALYTICAL METHOD CESAT

AMBIENT TEMPERATURE 74

OPERATOR JSM

*Run 2*  
*Feldspar*

GAS	1		2		3		AVERAGE NET VOLUME	MULTIPLIER	MOLECULAR WEIGHT OF STACK GAS-DRY BASIS Mg lb/lb-mole
	ACTUAL READING	NET	ACTUAL READING	NET	ACTUAL READING	NET			
CO <sub>2</sub>	1.3	1.3	1.3	1.3			1.30	144/100	.572
O <sub>2</sub> (NET IS ACTUAL O <sub>2</sub> READING MINUS ACTUAL CO <sub>2</sub> )	19.6	18.3	19.5	18.2			18.25	32/100	5.84
CO (NET IS ACTUAL CO READING MINUS ACTUAL O <sub>2</sub> )	19.6	0.0	19.5	0.0			0.00	28/100	
N <sub>2</sub> (NET IS 100 MINUS ACTUAL CO)							80.45	28/100	22.526
								TOTAL	28.94

ORSEAT ANALYSIS AND DRY MOLECULAR WEIGHT DETERMINATION  
 COMMENTS:

PLANT Feldspar Corp PH #2

DATE 5/16/79

SAMPLING TIME (24-hr. CLOCK) 1420 - 1531

SAMPLING LOCATION 5th

SAMPLE TYPE (BAG, INTEGRATED, CONTINUOUS) ORSEAT

ANALYTICAL METHOD 78

AMBIENT TEMPERATURE JSM

OPERATOR

*Run 3*

GAS	1		2		3		AVERAGE NET VOLUME	MULTIPLIER	MOLECULAR WEIGHT OF STACK GAS-DRY BASIS M <sub>d</sub> lb/lb-mole	
	ACTUAL READING	NET	ACTUAL READING	NET	ACTUAL READING	NET				
CO <sub>2</sub>	19.6	1.6	19.5	1.5			1.55	144/100	1692	
O <sub>2</sub> (NET IS ACTUAL O <sub>2</sub> READING MINUS ACTUAL CO <sub>2</sub> )	19.6	18.0	19.5	18.0			18.00	32/100	5176	
CO (NET IS ACTUAL CO READING MINUS ACTUAL O <sub>2</sub> )	19.6	0.0	19.5	0.0			0.00	28/100		
N <sub>2</sub> (NET IS 100 MINUS ACTUAL CO)							80.45	28/100	22,576	
								TOTAL		28,960

PARTICULATE CLEANUP SHEET

PLANT Feldspar PH #2  
 DATE 5/16/79  
 OPERATOR JSM  
 RUN NUMBER 1 SAMPLE BOX NO. 1  
 BAR. PRESSURE 27.84 AMBIENT TEMP. 68°F  
 ACETONE BLANK VOL. 150 ml ACETONE WASH VOL. 150 ml  
 ACETONE BLANK CONCENTRATION, mg/mg —  
 ACETONE WASH BLANK, mg 1.00

CONTAINER NUMBER	WEIGHT OF PARTICULATE COLLECTED, mg		
	FINAL WEIGHT	TARE WEIGHT	WEIGHT GAIN
1 10	482.33	453.84	28.49
2	82,174.35	82,161.54	12.81
TOTAL	<del>                    </del>	<del>                    </del>	41.30
Less acetone blank			1.00
Weight of particulate matter			40.30

H <sub>2</sub> O Cont. No. <u>1-1</u>	VOLUME OF LIQUID WATER COLLECTED	
	IMPINGER VOLUME, ml	SILICA GEL WEIGHT, g
FINAL	237.0	209.2
INITIAL	200.0	200.0
LIQUID COLLECTED	37.0	9.2
TOTAL VOL COLLECTED	46.2	g*   ml

CONVERT WEIGHT OF WATER TO VOLUME BY DIVIDING TOTAL WEIGHT INCREASE BY DENSITY OF WATER (1 g/ml).

$$\frac{\text{INCREASE, g}}{1 \text{ g/ml}} = \text{VOLUME WATER, ml}$$

ADDITIONAL NOTES AND COMMENTS:

PARTICULATE CLEANUP SHEET

PLANT Feldspar PH #2  
 DATE 5/16/79  
 OPERATOR JSM  
 RUN NUMBER 2 SAMPLE BOX NO. 2  
 BAR. PRESSURE 27.84 AMBIENT TEMP. 74  
 ACETONE BLANK VOL. 150 ml ACETONE WASH VOL. 150 ml  
 ACETONE BLANK CONCENTRATION, mg/mg —  
 ACETONE WASH BLANK, mg 1.00

CONTAINER NUMBER	WEIGHT OF PARTICULATE COLLECTED, mg		
	FINAL WEIGHT	TARE WEIGHT	WEIGHT GAIN
1 13	477.99	449.95	28.04
2	98,981.12	98,972.24	8.88
TOTAL	<del>                    </del>	<del>                    </del>	36.92
Less acetone blank			1.00
Weight of particulate matter			35.92

H <sub>2</sub> O Cont. No. <u>1-2</u>	VOLUME OF LIQUID WATER COLLECTED	
	EMPIRICAL VOLUME, ml	SILICA GEL WEIGHT, g
FINAL	237.0	208.3
INITIAL	200.0	200.0
LIQUID COLLECTED	37.0	8.3
TOTAL VOL COLLECTED	45.3	g* ml

CONVERT WEIGHT OF WATER TO VOLUME BY DIVIDING TOTAL WEIGHT INCREASE BY DENSITY OF WATER (1 g/ml).

$$\frac{\text{INCREASE, g}}{1 \text{ g/ml}} = \text{VOLUME WATER, ml}$$

ADDITIONAL NOTES AND COMMENTS:

PARTICULATE CLEANUP SHEET

PLANT Teldspar Corp PH. #2

DATE 5/16/79

OPERATOR JSM

RUN NUMBER 3 SAMPLE BOX NO. 3

BAR. PRESSURE 27.84 AMBIENT TEMP. 78°F

ACETONE BLANK VOL. 150 ml ACETONE WASH VOL. 150 ml

ACETONE BLANK CONCENTRATION, mg/mg       

ACETONE WASH BLANK, mg 1.00

CONTAINER NUMBER	WEIGHT OF PARTICULATE COLLECTED, mg		
	FINAL WEIGHT	TARE WEIGHT	WEIGHT GAIN
1 12	479.67	451.29	28.38
2	99,487.02	99,460.19	26.83
TOTAL	<del>      </del>	<del>      </del>	54.61
Less acetone blank			1.00
Weight of particulate matter			53.61

H <sub>2</sub> O Cont. No. <u>1-3</u>	VOLUME OF LIQUID WATER COLLECTED	
	MEPHER VOLUME, ml	SILICA GEL WEIGHT, g
	FINAL	237.0
	INITIAL	200.0
	LIQUID COLLECTED	37.0
	TOTAL VOL COLLECTED	48.8
		g* ml

CONVERT WEIGHT OF WATER TO VOLUME BY DIVIDING TOTAL WEIGHT INCREASE BY DENSITY OF WATER (1 g/ml).

$$\frac{\text{INCREASE, g}}{1 \text{ g/ml}} = \text{VOLUME WATER, ml}$$

ADDITIONAL NOTES AND COMMENTS:

TEST PARTICIPANTS

James S. McCormack, P. E.

President  
Environmental Testing, Inc.

Guy Pushee

Technician  
Environmental Testing, Inc.

THURSDAY, AUGUST 18, 1977  
PART II



---

**ENVIRONMENTAL  
PROTECTION  
AGENCY**

■

**STANDARDS OF  
PERFORMANCE FOR NEW  
STATIONARY SOURCES**

**Revision to Reference Method 1-8**

Environmental Protection Agency

have peroxide impurities that will cause erroneously high sulfuric acid mist measurements, a test for peroxides in isopropanol has been included in the method.

4. The gravimetric technique for moisture content (rather than volumetric) has been specified because a mixture of isopropyl alcohol and water will have a volume less than the sum of the volumes of its content.

5. A closer correspondence has been made between similar parts of Methods 8 and 5.

MISCELLANEOUS

Several commenters questioned the meaning of the term "subject to the approval of the Administrator" in relation to using alternate test methods and procedures. As defined in § 80.2 of subpart A, the "Administrator" includes any authorized representative of the Administrator of the Environmental Protection Agency. Authorized representatives are EPA officials in EPA Regional Offices or State, local, and regional governmental officials who have been delegated the responsibility of enforcing regulations under 40 CFR 60. These officials in consultation with other staff members familiar with technical aspects of source testing will render decisions regarding acceptable alternate test procedures.

In accordance with section 117 of the Act, publication of these methods was preceded by consultation with appropriate advisory committees, independent experts, and Federal departments and agencies.

(Secs. 111, 114 and 301(a) of the Clean Air Act, sec. 4(a) of Pub. L. No. 91-604, 84 Stat. 1683; sec. 4(a) of Pub. L. No. 91-604, 84 Stat. 1687; sec. 2 of Pub. L. No. 90-148, 81 Stat. 504 [42 U.S.C. 1857c-4, 1857c-9, 1857g(a)].)

Note.—The Environmental Protection Agency has determined that this document does not contain a major proposal requiring preparation of an Economic Impact Analysis under Executive Orders 11821 and 11949 and OMB Circular A-107.

Dated: August 10, 1977.

DOUGLAS M. COSTLE,  
Administrator.

Part 80 of Chapter I of Title 40 of the Code of Federal Regulations is amended by revising Methods 1 through 8 of Appendix A—Reference Methods as follows:

APPENDIX A—REFERENCE METHODS

The reference methods in this appendix are referred to in § 60.8 (Performance Tests) and § 60.11 (Compliance With Standards and Maintenance Requirements) of 40 CFR Part 60, Subpart A (General Provisions). Specific uses of these reference methods are described in the standards of performance contained in the subparts, beginning with Subpart D.

Within each standard of performance, a section titled "Test Methods and Procedures" is provided to (1) identify the test methods applicable to the facility subject to the respective standard and (2) identify any special instructions or conditions to be followed when applying a method to the respective facility. Such instructions (for example, establish sampling rates, volumes, or temperatures) are to be used either in addition to, or as a substitute for procedures in a reference method. Similarly, for sources subject to emission monitoring requirements, specific instructions pertaining to any use of a reference method are provided in the subpart or in Appendix B.

Inclusion of methods in this appendix is not intended as an endorsement or denial of their applicability to sources that are not subject to standards of performance. The methods are potentially applicable to other sources; however, applicability should be confirmed by careful and appropriate evaluation of the conditions prevalent at such sources.

The approach followed in the formulation of the reference methods involves specifications for equipment, procedures, and performance. In concept, a performance specification approach would be preferable in all methods because this allows the greatest flexibility to the user. In practice, however, this approach is impractical in most cases because performance specifications cannot be established. Most of the methods described herein, therefore, involve specific equipment specifications and procedures, and only a few methods in this appendix rely on performance criteria.

Minor changes in the reference methods should not necessarily affect the validity of the results and it is recognized that alternative and equivalent methods exist. Section 60.1 provides authority for the Administrator to specify or approve (1) equivalent methods, (2) alternative methods, and (3) minor changes in the methodology of the reference methods. It should be clearly understood that unless otherwise identified all such methods and changes must have prior approval of the Administrator. An owner employing such methods or deviations from the reference methods without obtaining prior approval does so at the risk of subsequent disapproval and retesting with approved methods.

Within the reference methods, certain specific equipment or procedures are recognized as being acceptable or potentially acceptable and are specifically identified in the methods. The items identified as acceptable options may be used without approval but must be identified in the test report. The potentially approvable options are cited as "subject to the approval of the Administrator" or as "or equivalent." Such potentially approvable techniques or alternatives may be used at the discretion of the owner without prior approval. However, detailed descriptions for applying these potentially approvable techniques or alternatives are not provided in the reference methods. Also, the potentially approvable options are not necessarily acceptable in all applications. Therefore, an owner electing to use such potentially approvable techniques or alternatives is responsible for: (1) assuring that the techniques or alternatives are in fact applicable and are properly executed; (2) including a written description of the alternative method in the test report (the written method must be clear and must be capable of being performed without additional instruction, and the degree of detail should be similar to the detail contained in the reference method); and (3) providing any rationale or supporting data necessary to show the validity of the alternative in the particular application. Failure to meet these requirements can result in the Administrator's disapproval of the alternative.

METHOD 1—SAMPLE AND VELOCITY TRAVERSAL FOR STATIONARY SOURCES

1. Principle and Applicability

1.1 Principle. To aid in the representative measurement of pollutant emissions and/or total volumetric flow rate from a stationary source, a measurement site where the effluent stream is flowing in a known direction is selected, and the cross-section of the stack is divided into a number of equal areas. A traverse point is then located within each of these equal areas.

1.2 Applicability. This method is applicable to flowing gas streams in ducts, stacks, and flues. The method cannot be used when: (1) flow is cyclonic or swirling (see Section 2.4); (2) a stack is smaller than about 0.30 meter (12 in.) in diameter, or 0.371 m<sup>2</sup> (113 in.<sup>2</sup>) in cross-sectional area, or (3) the measurement site is less than two stack or duct diameters downstream or less than a half diameter upstream from a flow disturbance.

The requirements of this method must be considered before construction of a new facility from which emissions will be measured; failure to do so may require subsequent alterations to the stack or deviation from the standard procedure. Cases involving variants are subject to approval by the Administrator, U.S. Environmental Protection Agency.

2. Procedure

2.1 Selection of Measurement Site. Flaming or velocity measurement is performed at a site located at least eight stack or duct diameters downstream and two diameters upstream from any flow disturbance such as a bend, expansion, or contraction in the stack, or from a visible flare. If necessary, an alternative location may be selected, at a position at least two stack or duct diameters downstream and a half diameter upstream from any flow disturbance. For a rectangular cross section, an equivalent diameter ( $D_e$ ) shall be calculated from the following equation, to determine the upstream and downstream distances:

$$D_e = \frac{2LW}{L+W}$$

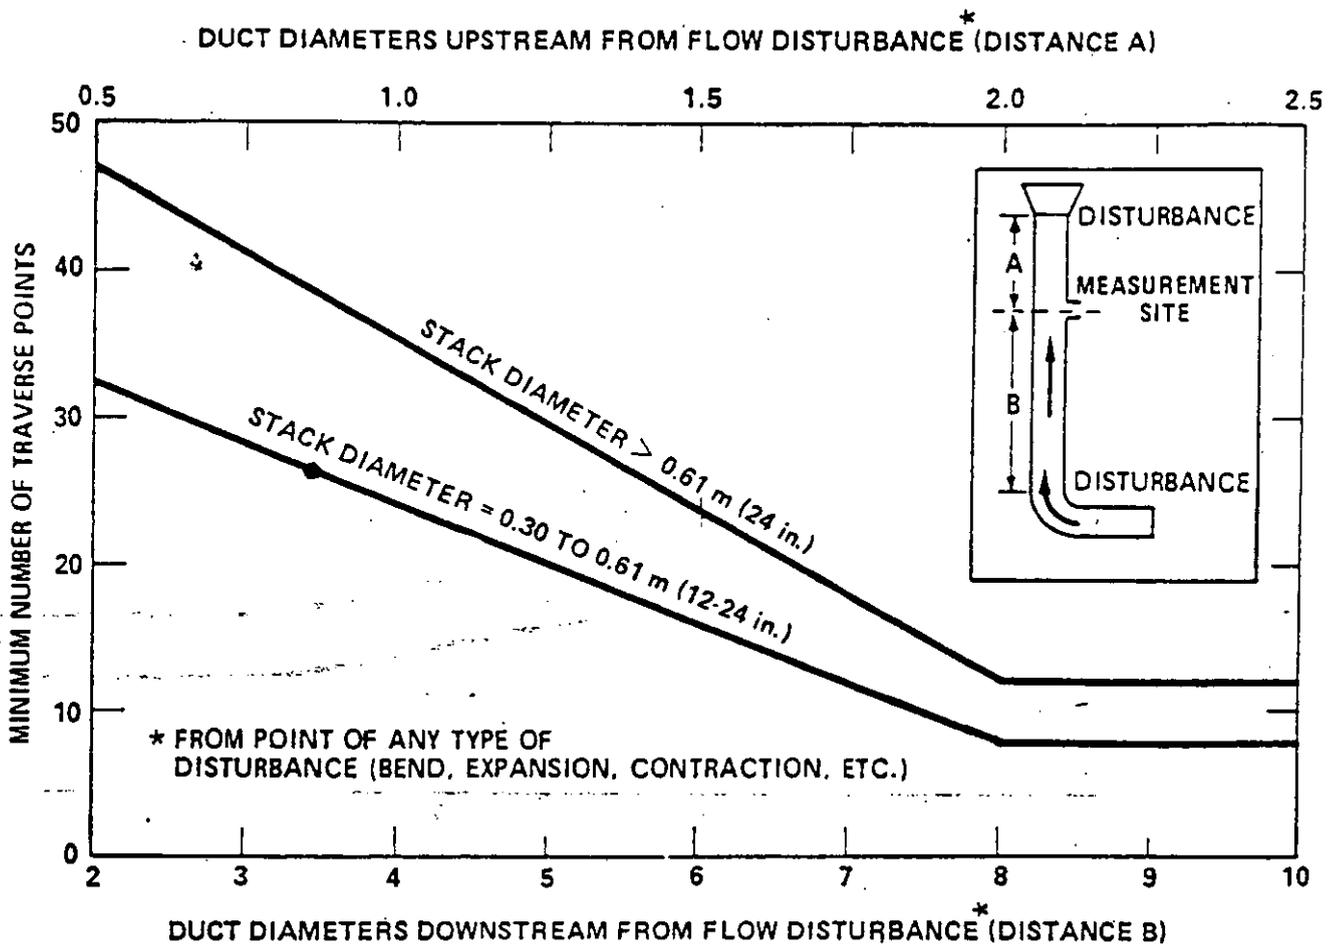


Figure 1-1. Minimum number of traverse points for particulate traverses.

where  $L$  = length and  $W$  = width.

2.2 Determining the Number of Traverse Points.

2.2.1 Particulate Traverses. When the eight- and two-diameter criterion can be met, the minimum number of traverse points shall be: (1) twelve, for circular or rectangular stacks with diameters (or equivalent diameters) greater than 0.61 meter (24 in.); (2) eight, for circular stacks with diameters between 0.30 and 0.61 meter (12-24 in.); (3) nine, for rectangular stacks with equivalent diameters between 0.30 and 0.61 meter (12-24 in.).

When the eight- and two-diameter criterion cannot be met, the minimum number of traverse points is determined from Figure 1-1. Before referring to the figure, however, determine the distances from the chosen measurement site to the nearest upstream and downstream disturbances, and divide each distance by the stack diameter or equivalent diameter, to determine the distance in terms of the number of duct diameters. Then, determine from Figure 1-1 the minimum number of traverse points that corresponds: (1) to the number of duct diameters upstream; and (2) to the number of diameters downstream. Select the higher of the two minimum numbers of traverse points, or a greater value, so that for circular stacks the number is a multiple of 4, and for rectangular stacks, the number is one of those shown in Table 1-1.

TABLE 1-1. Cross-sectional layout for rectangular stacks

Number of traverse points:	Matrix layout
9	3x3
12	4x3
16	4x4
20	5x4
25	5x5
30	6x5
36	6x6
42	7x6
49	7x7

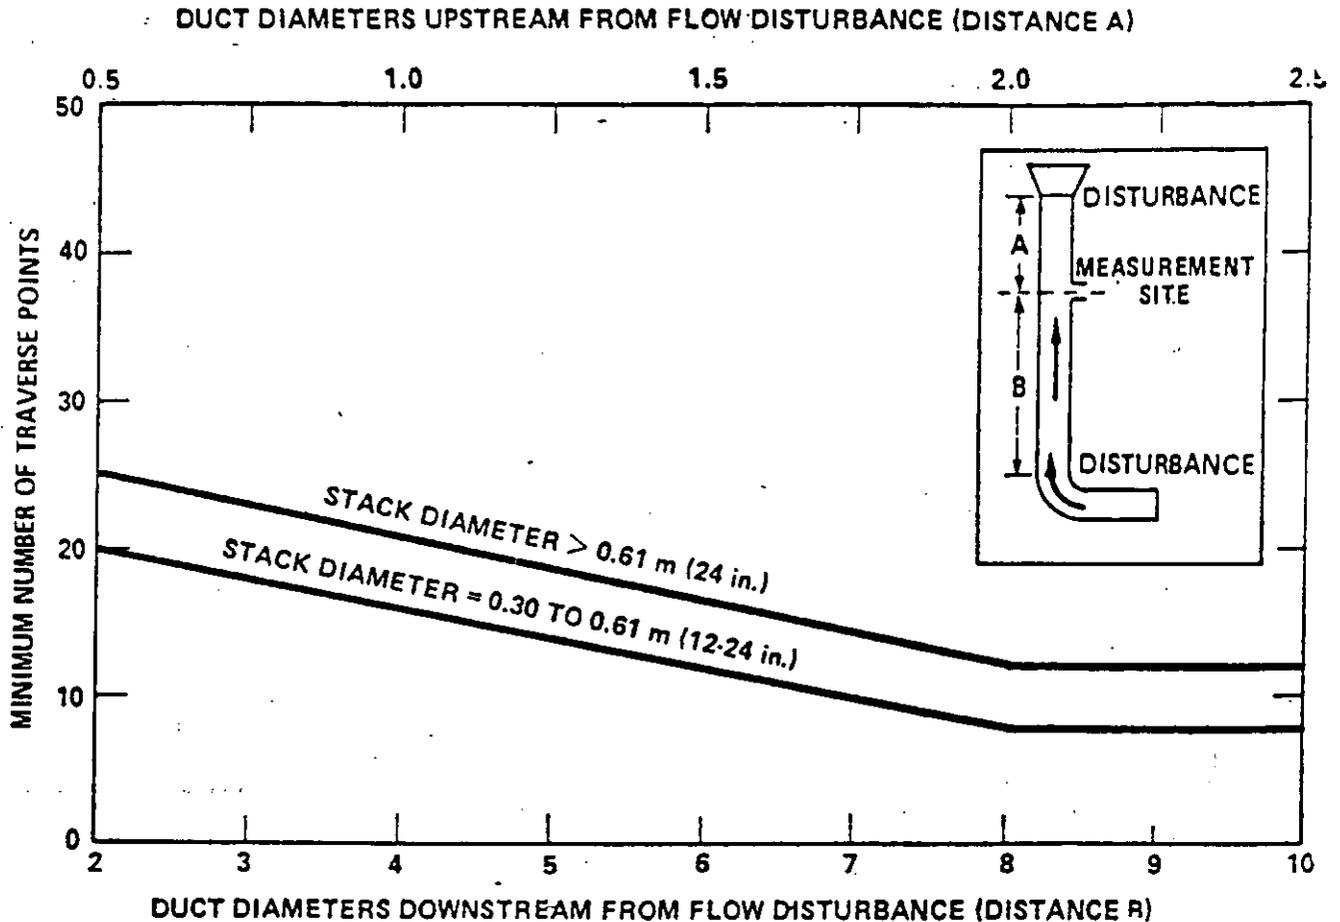


Figure 1-2. Minimum number of traverse points for velocity (nonparticulate) traverses.

2.2.2 Velocity (Non-Particulate) Traverses. When velocity or volumetric flow rate is to be determined (but not particulate matter), the same procedure as that for particulate traverses (Section 2.2.1) is followed, except that Figure 1-2 may be used instead of Figure 1-1.

2.3 Cross-Sectional Layout and Location of Traverse Points.

2.3.1 Circular Stacks. Locate the traverse points on two perpendicular diameters according to Table 1-2 and the example shown in Figure 1-3. Any equation (for examples, see Citations 2 and 3 in the Bibliography) that gives the same values as those in Table 1-2 may be used in lieu of Table 1-2.

For particulate traverses, one of the diameters must be in a plane containing the greatest expected concentration variation, e.g., after bends, one diameter shall be in the plane of the bend. This requirement becomes less critical as the distance from the disturbance increases; therefore, other diameter locations may be used, subject to approval of the Administrator.

In addition, for stacks having diameters greater than 0.61 m (24 in.), no traverse points shall be located within 2.5 centimeters (1.00 in.) of the stack walls; and for stack diameters equal to or less than 0.61 m (24 in.), no traverse points shall be located within 1.3 cm (0.50 in.) of the stack walls. To meet these criteria, observe the procedures given below.

2.3.1.1 Stacks With Diameters Greater Than 0.61 m (24 in.). When any of the traverse points as located in Section 2.3.1 fall within 2.5 cm (1.00 in.) of the stack walls, relocate them away from the stack walls to: (1) a distance of 2.5 cm (1.00 in.); or (2) a distance equal to the nozzle inside diameter, whichever is larger. These relocated traverse points (on each end of a diameter) shall be the "adjusted" traverse points.

Whenever two successive traverse points are combined to form a single adjusted traverse point, treat the adjusted point as two separate traverse points, both in the sampling (or velocity measurement) procedure, and in recording the data.

RULES AND REGULATIONS

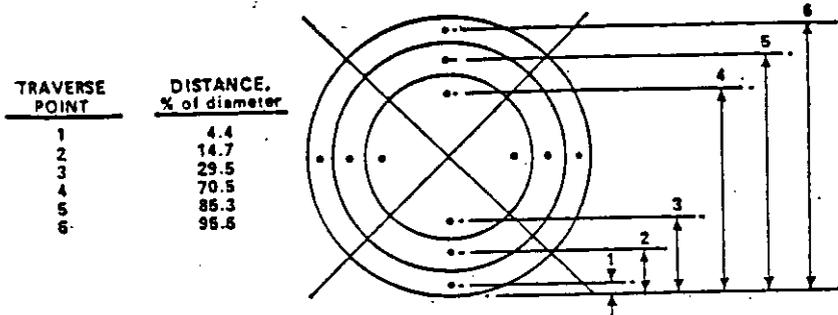


Figure 1-3. Example showing circular stack cross section divided into 12 equal areas, with location of traverse points indicated.

(2) In stacks having tangential inlets or other duct configurations which tend to induce swirling; in these instances, the presence or absence of cyclonic flow at the sampling location must be determined. The following techniques are acceptable for this determination.

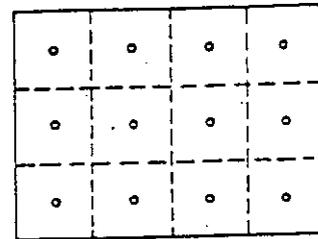


Figure 1-4. Example showing rectangular stack cross section divided into 12 equal areas, with a traverse point at centroid of each area.

Table 1-2. LOCATION OF TRAVERSE POINTS IN CIRCULAR STACKS (Percent of stack diameter from inside wall to traverse point)

Traverse point number on a diameter	Number of traverse points on a diameter											
	2	4	6	8	10	12	14	16	18	20	22	24
1	14.6	6.7	4.4	3.2	2.6	2.1	1.8	1.6	1.4	1.3	1.1	1.1
2	85.4	25.0	14.6	10.5	8.2	6.7	5.7	4.9	4.4	3.9	3.5	3.2
3		75.0	29.6	19.4	14.6	11.8	9.9	8.5	7.5	6.7	6.0	5.5
4		93.3	70.4	32.3	22.6	17.7	14.6	12.5	10.9	9.7	8.7	7.9
5			85.4	67.7	34.2	25.0	20.1	16.9	14.6	12.9	11.6	10.5
6			95.6	80.6	65.8	35.6	26.9	22.0	18.8	16.5	14.6	13.2
7				89.5	77.4	64.4	36.6	28.3	23.6	20.4	18.0	16.1
8				96.8	85.4	75.0	63.4	37.5	29.6	25.0	21.8	19.4
9					91.8	82.3	73.1	62.5	38.2	30.6	26.2	23.0
10					97.4	88.2	79.9	71.7	61.8	38.8	31.5	27.2
11						93.3	85.4	78.0	70.4	61.2	39.3	32.3
12						97.9	90.1	83.1	76.4	69.4	60.7	39.8
13							94.3	87.5	81.2	75.0	68.5	60.2
14							98.2	91.5	85.4	79.6	73.8	67.7
15								95.1	89.1	83.5	78.2	72.8
16								98.4	92.5	87.1	82.0	77.0
17									95.6	90.3	85.4	80.6
18									98.6	93.3	88.4	83.9
19										96.1	91.3	86.8
20										98.7	94.0	89.5
21											96.5	92.1
22											98.9	94.5
23												96.8
24												98.9

2.2.1.2 Stacks With Diameters Equal to or Less Than 0.61 m (24 in.). Follow the procedure in Section 2.3.1.1, noting only that any "adjusted" points should be relocated away from the stack walls to: (1) a distance of 1.3 cm (0.50 in.); or (2) a distance equal to the nozzle inside diameter, whichever is larger.

2.3.2 Rectangular Stacks. Determine the number of traverse points as explained in Sections 2.1 and 2.2 of this method. From Table 1-1, determine the grid configuration. Divide the stack cross-section into as many equal rectangular elemental areas as traverse points,

and then locate a traverse point at the centroid of each equal area according to the example in Figure 1-4.

The situation of traverse points being too close to the stack walls is not expected to arise with rectangular stacks. If this problem should ever arise, the Administrator must be contacted for resolution of the matter.

2.4 Verification of Absence of Cyclonic Flow. In most stationary sources, the direction of stack gas flow is essentially parallel to the stack walls. However, cyclonic flow may exist (1) after such devices as cyclones and inertial demisters following venturi scrubbers, or

Level and zero the manometer. Connect a Type S pitot tube to the manometer. Position the Type S pitot tube at each traverse point, in succession, so that the planes of the face openings of the pitot tube are perpendicular to the stack cross-sectional plane; when the Type S pitot tube is in this position, it is at "0° reference." Note the differential pressure ( $\Delta p$ ) reading at each traverse point. If a null (zero) pitot reading is obtained at 0° reference at a given traverse point, an acceptable flow condition exists at that point. If the pitot reading is not zero at 0° reference, rotate the pitot tube (up to a 90° yaw angle), until a null reading is obtained. Carefully determine and record the value of the rotation angle ( $\alpha$ ) to the nearest degree. After the null technique has been applied at each traverse point, calculate the average of the absolute values of  $\alpha$ ; assign a value of 0° to those points for which no rotation was required, and include these in the overall average. If the average value of  $\alpha$  is greater than 10°, the overall flow condition in the stack is unacceptable and alternative methodology, subject to the approval of the Administrator, must be used to perform accurate sample and velocity traverses.

2. Bibliography

1. Determining Dust Concentration in a Gas Stream. ASME. Performance Test Code No. 27. New York, 1957.
2. Devorkin, Howard, et al. Air Pollution Source Testing Manual. Air Pollution Control District. Los Angeles, CA. November 1963.
3. Methods for Determination of Velocity, Volume, Dust and Mist Content of Gases. Western Precipitation Division of Joy Manufacturing Co. Los Angeles, CA. Bulletin WP-50. 1968.
4. Standard Method for Sampling Stacks for Particulate Matter. In: 1971 Book of ASTM Standards, Part 23. ASTM Designation D-2925-71. Philadelphia, Pa. 1971.
5. Hanson, H. A., et al. Particulate Sampling Strategies for Large Power Plants Including Nonuniform Flow. USEPA, O.R.D., ESRL, Research Triangle Park, N.C. EPA-600/3-76-170, June 1976.
6. Entropy Environmentalists, Inc. Determination of the Optimum Number of Sampling Points: An Analysis of Method 1 Criteria. Environmental Protection Agency, Research Triangle Park, N.C. EPA Contract No. 68-01-3172, Task 7.

METHOD 2—DETERMINATION OF STACK GAS VELOCITY AND VOLUMETRIC FLOW RATE (TYPE S PITOT TUBE)

1. Principle and Applicability

1.1 Principle. The average gas velocity in a stack is determined from the gas density and from measurement of the average velocity head with a Type S (Stauscheibe or reverse type) pitot tube.

1.2 Applicability. This method is applicable for measurement of the average velocity of a gas stream and for quantifying gas flow.

This procedure is not applicable at measurement sites which fail to meet the criteria of Method 1, Section 2.1. Also, the method cannot be used for direct measurement in cyclonic or swirling gas streams; Section 2.4 of Method 1 shows how to determine cyclonic or swirling flow conditions. When unacceptable conditions exist, alternative procedures, subject to the approval of the Administrator, U.S. Environmental Protection Agency, must be employed to make accurate flow rate determinations; examples of such alternative procedures are: (1) to install straightening vanes; (2) to calculate the total volumetric flow rate stoichiometrically, or (3) to move to another measurement site at which the flow is acceptable.

2. Apparatus

Specifications for the apparatus are given below. Any other apparatus that has been demonstrated (subject to approval of the Administrator) to be capable of meeting the specifications will be considered acceptable.

**RULES AND REGULATIONS**

3.6 Determine the stack gas dry molecular weight. For combustion processes or processes that emit essentially CO<sub>2</sub>, O<sub>2</sub>, CO, and N<sub>2</sub>, use Method 3. For processes emitting essentially air, an analysis need not be conducted; use a dry molecular weight of 29.0. For other processes, other methods, subject to the approval of the Administrator, must be used.

3.7 Obtain the moisture content from Reference Method 4 (or equivalent) or from Method 5.

3.8 Determine the cross-sectional area of the stack or duct at the sampling location. Whenever possible, physically measure the stack dimensions rather than using blueprints.

**4. Calibration**

4.1 Type 8 Pitot Tube. Before its initial use, carefully examine the Type 8 pitot tube in top, side, and end views to verify that the face openings of the tube are aligned within the specifications illustrated in Figure 2-3 or 2-4. The pitot tube shall not be used if it fails to meet these alignment specifications.

After verifying the face opening alignment, measure and record the following dimensions of the pitot tube:


(a) the external tubing diameter (dimension D<sub>t</sub>, Figure 2-2b); and (b) the base-to-opening plane distance (dimensions P<sub>1</sub> and P<sub>2</sub>, Figure 2-2b). If D<sub>t</sub> is between 0.48 and 0.96 cm (3/16 and 3/8 in.) and if P<sub>1</sub> and P<sub>2</sub> are equal and between 1.05 and 1.50 R<sub>n</sub>, there are two possible options: (1) the pitot tube may be calibrated according to the procedure outlined in Sections 4.1.2 through 4.1.5 below, or (2) a baseline (isolated tube) coefficient 0.84 may be assigned to the pitot tube. Note, however, that if the pitot tube is part of an assembly, calibration may still be required, despite knowledge of the baseline coefficient value (see Section 4.1.1). If D<sub>t</sub>, P<sub>1</sub>, and P<sub>2</sub> are outside the specified limits, the pitot tube must be calibrated as outlined in 4.1.2 through 4.1.5 below.

4.1.1 Type 8 Pitot Tube Assemblies. During sample and velocity traverses, the isolated Type 8 pitot tube is not always used; in many instances, the pitot tube is used in combination with other source-sampling components (thermocouple, sampling probe, nozzle) as part of an "assembly." The presence of other sampling components can sometimes affect the baseline value of the Type 8 pitot tube coefficient (Citation 9 in Section 6); therefore an assigned (or otherwise known) baseline coefficient

value may or may not be valid for a given assembly. The baseline and assembly coefficient values will be identical only when the relative placement of the components in the assembly is such that aerodynamic interference effects are eliminated. Figures 2-5 through 2-8 illustrate interference-free component arrangements for Type 8 pitot tubes having external diameters for Type 8 pitot tubes that fall to meet any or all of the specifications of Figures 2-5 through 2-8 shall be calibrated according to the procedure outlined in Sections 4.1.2 through 4.1.5 below, and prior to calibration, the values of the inter-component spacings (pitot-nozzle, pitot-thermocouple, pitot-probe sheath) shall be measured and recorded.

Note.—Do not use any Type 8 pitot tube assembly which is constructed such that the impact pressure opening plane of the pitot tube is below the entry plane of the nozzle (see Figure 2-6b).

4.1.2 Calibration Setup. If the Type 8 pitot tube is to be calibrated, one leg of the tube shall be permanently marked A, and the other, B. Calibration shall be done in a flow system having the following essential design features:

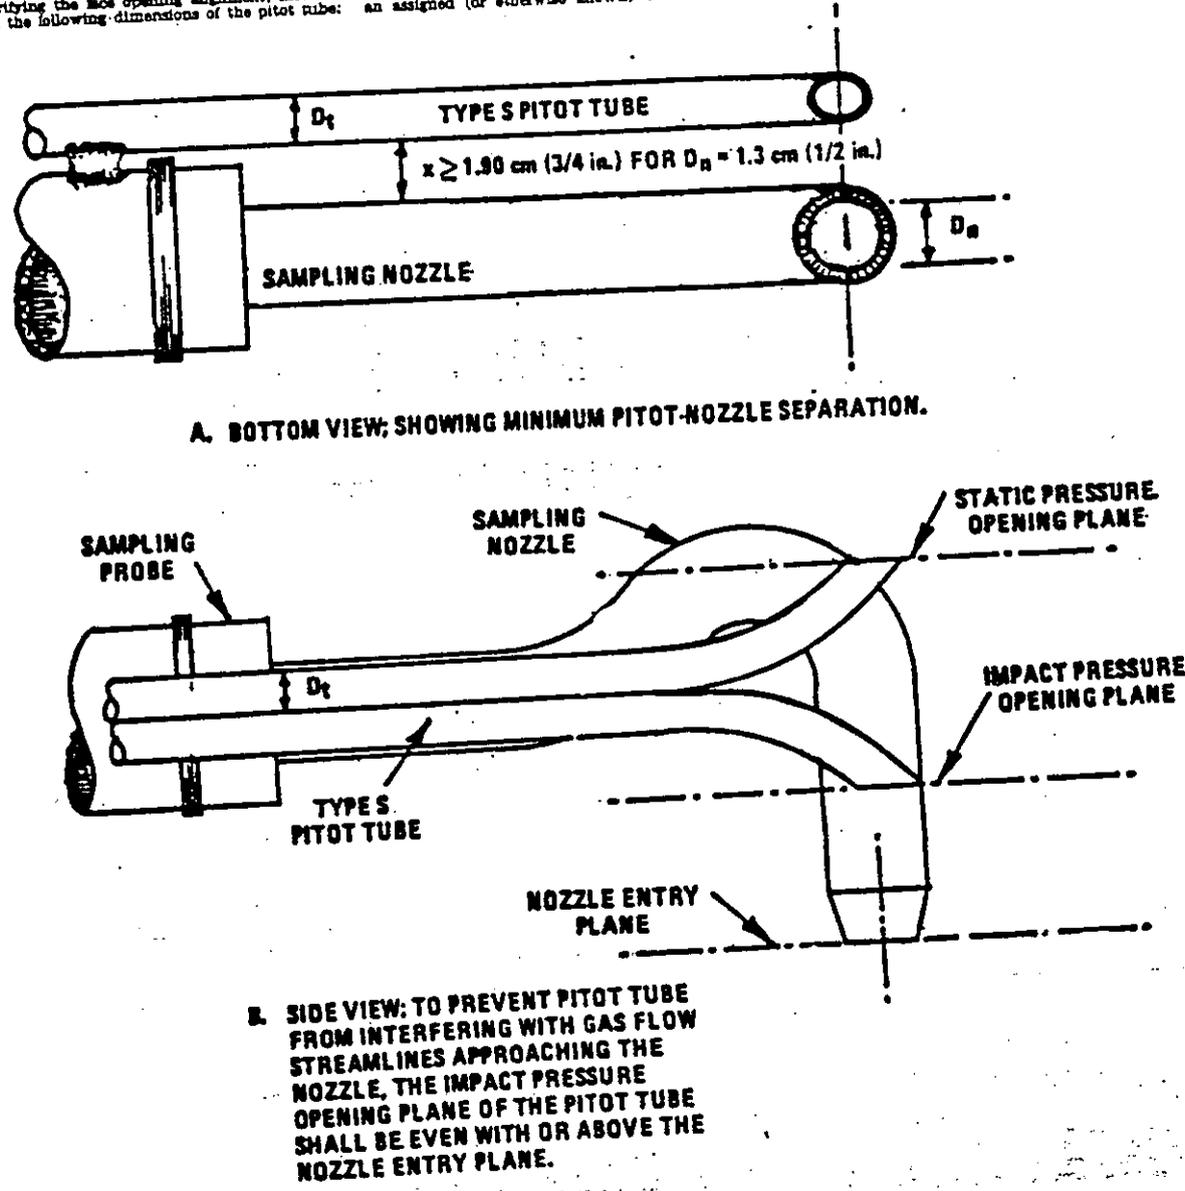

**A. BOTTOM VIEW; SHOWING MINIMUM PITOT-NOZZLE SEPARATION.**

**B. SIDE VIEW: TO PREVENT PITOT TUBE FROM INTERFERING WITH GAS FLOW STREAMLINES APPROACHING THE NOZZLE, THE IMPACT PRESSURE OPENING PLANE OF THE PITOT TUBE SHALL BE EVEN WITH OR ABOVE THE NOZZLE ENTRY PLANE.**

**Figure 2-6. Proper pitot tube - sampling nozzle configuration to prevent aerodynamic interference; buttonhook - type nozzle; centers of nozzle and pitot opening aligned; D<sub>t</sub> between 0.48 and 0.95 cm (3/16 and 3/8 in.).**

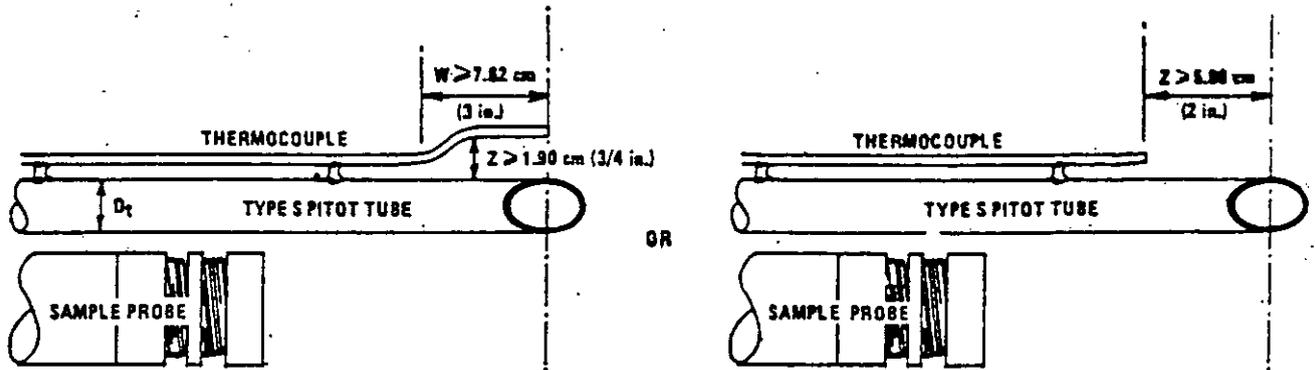


Figure 2-7. Proper thermocouple placement to prevent interference;  $D_t$  between 0.48 and 0.95 cm (3/16 and 3/8 in.).

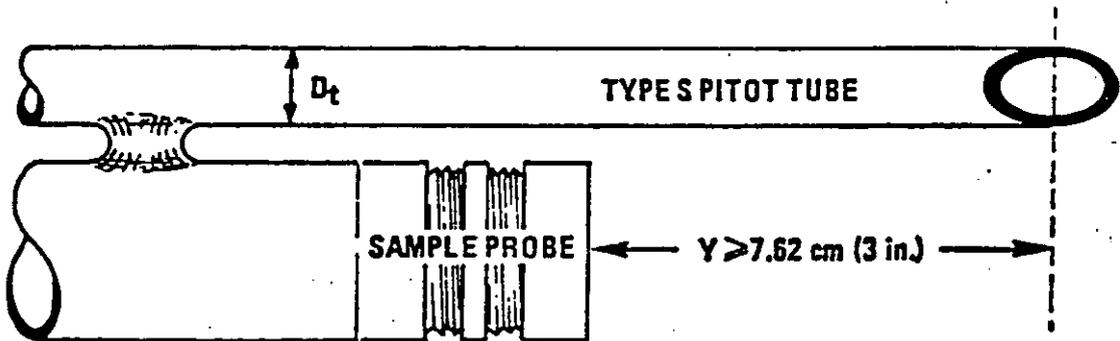


Figure 2-8. Minimum pitot-sample probe separation needed to prevent interference;  $D_t$  between 0.48 and 0.95 cm (3/16 and 3/8 in.).

4.1.2.1 The flowing gas stream must be confined to a duct of definite cross-sectional area, either circular or rectangular. For circular cross-sections, the minimum duct diameter shall be 30.5 cm (12 in.); for rectangular cross-sections, the width (shorter side) shall be at least 25.4 cm (10 in.).

4.1.2.2 The cross-sectional area of the calibration duct must be constant over a distance of 10 or more duct diameters. For a rectangular cross-section, use an equivalent diameter, calculated from the following equation, to determine the number of duct diameters:

$$D_e = \frac{2LW}{L+W}$$

Equation 2-1

where:

- $D_e$  = Equivalent diameter
- $L$  = Length
- $W$  = Width

To ensure the presence of stable, fully developed flow patterns at the calibration site, or "test section," the site must be located at least eight diameters downstream and two diameters upstream from the nearest disturbances.

NOTE.—The eight- and two-diameter criteria are not absolute; other test section locations may be used (subject to approval of the Administrator), provided that the flow at the test site is stable and demonstrably parallel to the duct axis.

4.1.2.3 The flow system shall have the capacity to generate a test-section velocity around 915 m/min (3,000

f/min). This velocity must be constant with time to guarantee steady flow during calibration. Note that Type S pitot tube coefficients obtained by single-velocity calibration at 915 m/min (3,000 f/min) will generally be valid to within  $\pm 3$  percent for the measurement of velocities above 306 m/min (1,000 f/min) and to within  $\pm 5$  percent for the measurement of velocities between 180 and 306 m/min (600 and 1,000 f/min). If a more precise correlation between  $C_p$  and velocity is desired, the flow system shall have the capacity to generate at least four distinct, time-invariant test-section velocities covering the velocity range from 180 to 1,525 m/min (600 to 5,000 f/min), and calibration data shall be taken at regular velocity intervals over this range (see Citations 9 and 14 in Section 6 for details).

4.1.2.4 Two entry ports, one each for the standard and Type S pitot tubes, shall be cut in the test section; the standard pitot entry port shall be located slightly downstream of the Type S port, so that the standard and Type S impact openings will lie in the same cross-sectional plane during calibration. To facilitate alignment of the pitot tubes during calibration, it is advisable that the test section be constructed of plexiglas or some other transparent material.

4.1.3 Calibration Procedure. Note that this procedure is a general one and must not be used without first referring to the special considerations presented in Section 4.1.5. Note also that this procedure applies only to single-velocity calibration. To obtain calibration data for the A and B sides of the Type S pitot tube, proceed as follows:

4.1.3.1 Make sure that the manometer is properly filled and that the oil is free from contamination and is of the proper density. Inspect and leak-check all pitot lines; repair or replace if necessary.

4.1.3.2 Level and zero the manometer. Turn on the fan and allow the flow to stabilize. Seal the Type S entry port.

4.1.3.3 Ensure that the manometer is level and zeroed. Position the standard pitot tube at the calibration point (determined as outlined in Section 4.1.3.1), and align the tube so that its tip is pointed directly into the flow. Particular care should be taken in aligning the tube to avoid yaw and pitch angles. Make sure that the entry port surrounding the tube is properly sealed.

4.1.3.4 Read  $\Delta p_s$  and record its value in a data table similar to the one shown in Figure 2-9. Remove the standard pitot tube from the duct and disconnect it from the manometer. Seal the standard entry port.

4.1.3.5 Connect the Type S pitot tube to the manometer. Open the Type S entry port. Check the manometer level and zero. Insert and align the Type S pitot tube so that its A side impact opening is at the same point as was the standard pitot tube and is pointed directly into the flow. Make sure that the entry port surrounding the tube is properly sealed.

4.1.3.6 Read  $\Delta p_s$  and enter its value in the data table. Remove the Type S pitot tube from the duct and disconnect it from the manometer.

4.1.3.7 Repeat steps 4.1.3.3 through 4.1.3.6 above until three pairs of  $\Delta p$  readings have been obtained.

4.1.3.8 Repeat steps 4.1.3.3 through 4.1.3.7 above for the B side of the Type S pitot tube.

4.1.3.9 Perform calculations, as described in Section 4.1.4 below.

4.1.4 Calculations.

4.1.4.1 For each of the six pairs of  $\Delta p$  readings (i.e., three from side A and three from side B) obtained in Section 4.1.3 above, calculate the value of the Type S pitot tube coefficient as follows:

PITOT TUBE IDENTIFICATION NUMBER: \_\_\_\_\_ DATE: \_\_\_\_\_  
 CALIBRATED BY: \_\_\_\_\_

"A" SIDE CALIBRATION				
RUN NO.	$\Delta P_{std}$ cm H <sub>2</sub> O (in. H <sub>2</sub> O)	$\Delta P(s)$ cm H <sub>2</sub> O (in. H <sub>2</sub> O)	$C_p(s)$	DEVIATION $C_p(s) - \bar{C}_p(A)$
1				
2				
3				
			$\bar{C}_p$ (SIDE A)	

"B" SIDE CALIBRATION				
RUN NO.	$\Delta P_{std}$ cm H <sub>2</sub> O (in. H <sub>2</sub> O)	$\Delta P(s)$ cm H <sub>2</sub> O (in. H <sub>2</sub> O)	$C_p(s)$	DEVIATION $C_p(s) - \bar{C}_p(B)$
1				
2				
3				
			$\bar{C}_p$ (SIDE B)	

$$\text{AVERAGE DEVIATION} = \sigma (A \text{ OR } B) = \frac{\sum |C_p(s) - \bar{C}_p(A \text{ OR } B)|}{3} \leftarrow \text{MUST BE } < 0.01$$

$$|\bar{C}_p(\text{SIDE A}) - \bar{C}_p(\text{SIDE B})| \leftarrow \text{MUST BE } < 0.01$$

Figure 2-9. Pitot tube calibration data.

$$C_{p(s)} = C_{p(std)} \sqrt{\frac{\Delta P_{std}}{\Delta P_s}}$$

Equation 2-2

where:  
 $C_{p(s)}$  = Type S pitot tube coefficient  
 $C_{p(std)}$  = Standard pitot tube coefficient; use 0.99 if the coefficient is unknown and the tube is designed

according to the criteria of Sections 2.7.1 to 2.7.5 of this method.

$\Delta P_{std}$  = Velocity head measured by the standard pitot tube, cm H<sub>2</sub>O (in. H<sub>2</sub>O)  
 $\Delta P_s$  = Velocity head measured by the Type S pitot tube, cm H<sub>2</sub>O (in. H<sub>2</sub>O)

4.1.4.3 Calculate  $\bar{C}_p$  (side A), the mean A-side coefficient and  $\bar{C}_p$  (side B), the mean B-side coefficient; calculate the difference between these two average values.

4.1.4.3 Calculate the deviation of each of the three A-side values of  $C_{p(s)}$  from  $\bar{C}_p$  (side A), and the deviation of each B-side value of  $C_{p(s)}$  from  $\bar{C}_p$  (side B). Use the following equation:

$$\text{Deviation} = C_{p(s)} - \bar{C}_p(A \text{ or } B)$$

Equation 2-3

4.1.4.4 Calculate  $\sigma$ , the average deviation from the mean, for both the A and B sides of the pitot tube. Use the following equation:

$$\sigma (\text{side A or B}) = \frac{\sum |C_{p(s)} - \bar{C}_p(A \text{ or } B)|}{3}$$

Equation 2-4

4.1.4.5 Use the Type S pitot tube only if the values of  $\sigma$  (side A) and  $\sigma$  (side B) are less than or equal to 0.01 and if the absolute value of the difference between  $\bar{C}_p$  (A) and  $\bar{C}_p$  (B) is 0.01 or less.

4.1.5 Special considerations.

4.1.5.1 Selection of calibration point.  
 4.1.5.1.1 When an isolated Type S pitot tube is calibrated, select a calibration point at or near the center of the duct, and follow the procedures outlined in Sections 4.1.3 and 4.1.4 above. The Type S pitot coefficients so obtained, i.e.,  $\bar{C}_p$  (side A) and  $\bar{C}_p$  (side B), will be valid, so long as either: (1) the isolated pitot tube is used; or (2) the pitot tube is used with other components (nozzle, thermocouple, sample probe) in an arrangement that is free from aerodynamic interference effects (see Figures 2-6 through 2-8).

4.1.5.1.2 For Type S pitot tube-thermocouple combinations (without sample probe), select a calibration point at or near the center of the duct, and follow the procedures outlined in Sections 4.1.3 and 4.1.4 above. The coefficients so obtained will be valid so long as the pitot tube-thermocouple combination is used by itself or with other components in an interference-free arrangement (Figures 2-6 and 2-8).

4.1.5.1.3 For assemblies with sample probes, the calibration point should be located at or near the center of the duct; however, insertion of a probe sheath into a small duct may cause significant cross-sectional area blockage and yield incorrect coefficient values (Citation 9 in Section 6). Therefore, to minimize the blockage effect, the calibration point may be a few inches off-center if necessary. The actual blockage effect will be negligible when the theoretical blockage, as determined by a projected-area model of the probe sheath, is 2 percent or less of the duct cross-sectional area for assemblies without external sheaths (Figure 2-10a), and 3 percent or less for assemblies with external sheaths (Figure 2-10b).

4.1.5.2 For those probe assemblies in which pitot tube-nozzle interference is a factor (i.e., those in which the pitot-nozzle separation distance fails to meet the specification illustrated in Figure 2-6a), the value of  $C_{p(s)}$  depends upon the amount of free-space between the tube and nozzle, and therefore is a function of nozzle size. In these instances, separate calibrations shall be performed with each of the commonly used nozzle sizes in place. Note that the single-velocity calibration technique is acceptable for this purpose, even though the larger nozzle sizes (> 0.635 cm or 1/4 in.) are not ordinarily used for isokinetic sampling at velocities around 915 m/min (3,000 ft/min), which is the calibration velocity; note also that it is not necessary to draw an isokinetic sample during calibration (see Citation 19 in Section 6).

4.1.5.3 For a probe assembly constructed such that its pitot tube is always used in the same orientation, only one side of the pitot tube need be calibrated (the side which will face the flow). The pitot tube must still meet the alignment specifications of Figure 2-2 or 2-3, however, and must have an average deviation ( $\sigma$ ) value of 0.01 or less (see Section 4.1.4.4).

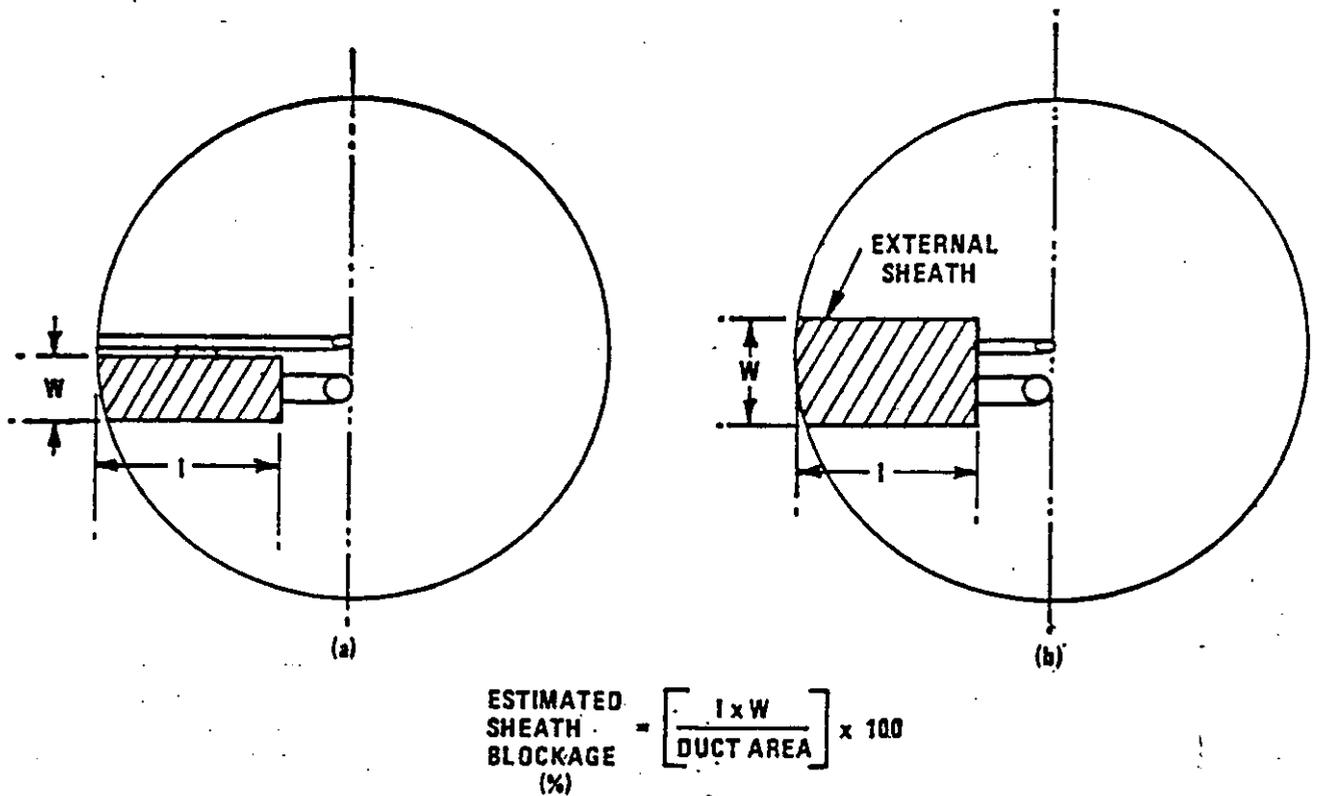


Figure 2-10. Projected-area models for typical pitot tube assemblies.

4.1.6 Field Use and Recalibration.

4.1.6.1 Field Use.

4.1.6.1.1 When a Type S pitot tube (isolated tube or assembly) is used in the field, the appropriate coefficient value (whether assigned or obtained by calibration) shall be used to perform velocity calculations. For calibrated Type S pitot tubes, the A side coefficient shall be used when the A side of the tube faces the flow, and the B side coefficient shall be used when the B side faces the flow; alternatively, the arithmetic average of the A and B side coefficient values may be used, irrespective of which side faces the flow.

4.1.6.1.2 When a probe assembly is used to sample a small duct (12 to 36 in. in diameter), the probe sheath sometimes blocks a significant part of the duct cross-section, causing a reduction in the effective value of  $C_p$ . Consult Citation 9 in Section 6 for details. Conventional pitot-sampling probe assemblies are not recommended for use in ducts having inside diameters smaller than 12 inches (Citation 16 in Section 6).

4.1.6.2 Recalibration.

4.1.6.2.1 Isolated Pitot Tubes. After each field use, the pitot tube shall be carefully reexamined in top, side, and end views. If the pitot face openings are still aligned within the specifications illustrated in Figure 2-2 or 2-3, it can be assumed that the baseline coefficient of the pitot tube has not changed. If, however, the tube has been damaged to the extent that it no longer meets the specifications of Figures 2-2 or 2-3, the damage shall either be repaired to restore proper alignment of the face openings or the tube shall be discarded.

4.1.6.2.2 Pitot Tube Assemblies. After each field use, check the face opening alignment of the pitot tube, as in Section 4.1.6.2.1; also, remeasure the intercomponent spacings of the assembly. If the intercomponent spacings have not changed and the face opening alignment is acceptable, it can be assumed that the coefficient of the assembly has not changed. If the face opening alignment is no longer within the specifications of Figures 2-2 or 2-3, either repair the damage or replace the pitot tube (calibrating the new assembly, if necessary). If the intercomponent spacings have changed, restore the original spacings or recalibrate the assembly.

4.2 Standard pitot tube (if applicable). If a standard pitot tube is used for the velocity traverse, the tube shall be constructed according to the criteria of Section 2.7 and shall be assigned a baseline coefficient value of 0.90. If the standard pitot tube is used as part of an assembly,

the tube shall be in an interference-free arrangement (subject to the approval of the Administrator).

4.3 Temperature Gauges. After each field use, calibrate dial thermometers, liquid-filled bulb thermometers, thermocouple-potentiometer systems, and other gauges at a temperature within 10 percent of the average absolute stack temperature. For temperatures up to 405° C (761° F), use an ASTM mercury-in-glass reference thermometer, or equivalent, as a reference; alternatively, either a reference thermocouple and potentiometer (calibrated by NBS) or thermometric fixed points, e.g., ice bath and boiling water (corrected for barometric pressure) may be used. For temperatures above 405° C (761° F), use an NBS-calibrated reference thermocouple-potentiometer system or an alternate reference, subject to the approval of the Administrator.

If, during calibration, the absolute temperatures measured with the gauge being calibrated and the reference gauge agree within 1.5 percent, the temperature data taken in the field shall be considered valid. Otherwise, the pollutant emission test shall either be considered invalid or adjustments (if appropriate) of the test results shall be made, subject to the approval of the Administrator.

4.4 Barometer. Calibrate the barometer used against a mercury barometer.

5. Calculations

Carry out calculations, retaining at least one extra decimal figure beyond that of the acquired data. Round off figures after final calculation.

5.1 Nomenclature.

- A = Cross-sectional area of stack, m<sup>2</sup> (ft<sup>2</sup>).
- B<sub>ws</sub> = Water vapor in the gas stream (from Method 5 or Reference Method 4), proportion by volume.
- C<sub>p</sub> = Pitot tube coefficient, dimensionless.
- K<sub>p</sub> = Pitot tube constant,

$$34.97 \frac{\text{m}}{\text{sec}} \left[ \frac{(\text{g/g-mole})(\text{mm Hg})}{(\text{°K})(\text{mm H}_2\text{O})} \right]^{1/2}$$

for the metric system and

$$85.49 \frac{\text{ft}}{\text{sec}} \left[ \frac{(\text{lb/lb-mole})(\text{in. Hg})}{(\text{°R})(\text{in. H}_2\text{O})} \right]^{1/2}$$

for the English system.

- M<sub>s</sub> = Molecular weight of stack gas, dry basis (see Section 3.4) g/g-mole (lb/lb-mole).
- M<sub>w</sub> = Molecular weight of stack gas, wet basis, g/g-mole (lb/lb-mole).

$$= M_s (1 - B_{ws}) + 18.0 B_{ws} \quad \text{Equation 2-3}$$

P<sub>ws</sub> = Barometric pressure at measurement site, mm Hg (in. Hg).

P<sub>s</sub> = Stack static pressure, mm Hg (in. Hg).

P<sub>t</sub> = Absolute stack gas pressure, mm Hg (in. Hg):

$$= P_{ws} + P_s \quad \text{Equation 2-4}$$

P<sub>std</sub> = Standard absolute pressure, 760 mm Hg (29.92 in. Hg).

Q<sub>sd</sub> = Dry volumetric stack gas flow rate corrected to standard conditions, dscm/hr (dscf/hr).

t<sub>s</sub> = Stack temperature, °C (°F).

T<sub>s</sub> = Absolute stack temperature, °K (°R).

$$= 273 + t_s \text{ for metric} \quad \text{Equation 2-7}$$

$$= 460 + t_s \text{ for English} \quad \text{Equation 2-8}$$

T<sub>std</sub> = Standard absolute temperature, 293 °K (52° R)

v<sub>s</sub> = Average stack gas velocity, m/sec (ft/sec).

Δp = Velocity head of stack gas, mm H<sub>2</sub>O (in. H<sub>2</sub>O):

3,600 = Conversion factor, sec/hr.

18.0 = Molecular weight of water, g/g-mole (lb-lb-mole).

5.2 Average stack gas velocity.

$$v_s = K_p C_p (\sqrt{\Delta p})^{0.95} \sqrt{\frac{T_s(\text{ave})}{P_s M_s}}$$

$$\quad \text{Equation 2-9}$$

5.3 Average stack gas dry volumetric flow rate.

$$Q_{sd} = 3,600 (1 - B_{ws}) v_s A \left( \frac{T_{std}}{T_s(\text{ave})} \right) \left( \frac{P_s}{P_{std}} \right)$$

$$\quad \text{Equation 2-10}$$

6. Bibliography

1. Mark, L. S. Mechanical Engineers' Handbook. New York, McGraw-Hill Book Co., Inc. 1961.
2. Perry, J. H. Chemical Engineers' Handbook. New York, McGraw-Hill Book Co., Inc. 1960.

3. Shicehara, R. T., W. F. Todd, and W. S. Smith. Significance of Errors in Stack Sampling Measurements. U.S. Environmental Protection Agency, Research Triangle Park, N.C. (Presented at the Annual Meeting of the Air Pollution Control Association, St. Louis, Mo., June 14-19, 1970.)
4. Standard Method for Sampling Stacks for Particulate Matter. In: 1971 Book of ASTM Standards, Part 23. Philadelphia, Pa. 1971. ASTM Designation D-2928-71.
5. Vennard, J. K. Elementary Fluid Mechanics. New York: John Wiley and Sons, Inc. 1947.
6. Fluid Meters—Their Theory and Application. American Society of Mechanical Engineers, New York, N.Y. 1959.
7. ASHRAE Handbook of Fundamentals. 1972, p. 208.
8. Annual Book of ASTM Standards, Part 23. 1974, p. 648.
9. Vollaro, R. F. Guidelines for Type S Pitot Tube Calibration. U.S. Environmental Protection Agency, Research Triangle Park, N.C. (Presented at 1st Annual Meeting, Source Evaluation Society, Dayton, Ohio, September 13, 1973.)
10. Vollaro, R. F. A Type S Pitot Tube Calibration Study. U.S. Environmental Protection Agency, Emission Measurement Branch, Research Triangle Park, N.C. July 1974.
11. Vollaro, R. F. The Effects of Impact Opening Misalignment on the Value of the Type S Pitot Tube Coefficient. U.S. Environmental Protection Agency, Emission Measurement Branch, Research Triangle Park, N.C. October 1976.
12. Vollaro, R. F. Establishment of a Baseline Coefficient Value for Properly Constructed Type S Pitot Tubes. U.S. Environmental Protection Agency, Emission Measurement Branch, Research Triangle Park, N.C. November 1976.
13. Vollaro, R. F. An Evaluation of Single-Velocity Calibration Techniques as a Means of Determining Type S Pitot Tube Coefficients. U.S. Environmental Protection Agency, Emission Measurement Branch, Research Triangle Park, N.C. August 1975.
14. Vollaro, R. F. The Use of Type S Pitot Tubes for the Measurement of Low Velocities. U.S. Environmental Protection Agency, Emission Measurement Branch, Research Triangle Park, N.C. November 1976.
15. Smith, Marvin L. Velocity Calibration of EPA Type Source Sampling Probe. United Technologies Corporation, Pratt and Whitney Aircraft Division, East Hartford, Conn. 1973.
16. Vollaro, R. F. Recommended Procedure for Sample Traverses in Ducts Smaller than 12 Inches in Diameter. U.S. Environmental Protection Agency, Emission Measurement Branch, Research Triangle Park, N.C. November 1976.
17. Ower, E. and R. C. Pankhurst. The Measurement of Air Flow, 4th Ed., London, Pergamon Press, 1964.
18. Vollaro, R. F. A Survey of Commercially Available Instrumentation for the Measurement of Low-Range Gas Velocities. U.S. Environmental Protection Agency, Emission Measurement Branch, Research Triangle Park, N.C. November 1976. (Unpublished Paper)
19. Gnyp, A. W., C. C. St. Pierre, D. S. Smith, D. Mosson, and J. Steiner. An Experimental Investigation of the Effect of Pitot Tube-Sampling Probe Configurations on the Magnitude of the S Type Pitot Tube Coefficient for Commercially Available Source Sampling

Probes. Prepared by the University of Windsor for the Ministry of the Environment, Toronto, Canada. February 1975.

#### METHOD 3—GAS ANALYSIS FOR CARBON DIOXIDE, OXYGEN, EXCESS AIR, AND DRY MOLECULAR WEIGHT

##### 1. Principle and Applicability

1.1 Principle. A gas sample is extracted from a stack, by one of the following methods: (1) single-point, grab sampling; (2) single-point, integrated sampling; or (3) multi-point, integrated sampling. The gas sample is analyzed for percent carbon dioxide (CO<sub>2</sub>), percent oxygen (O<sub>2</sub>), and, if necessary, percent carbon monoxide (CO). If a dry molecular weight determination is to be made, either an Orsat or a Fyrite analyzer may be used for the analysis; for excess air or emission rate correction factor determination, an Orsat analyzer must be used.

1.2 Applicability. This method is applicable for determining CO<sub>2</sub> and O<sub>2</sub> concentrations, excess air, and dry molecular weight of a sample from a gas stream of a fossil-fuel combustion process. The method may also be applicable to other processes where it has been determined that compounds other than CO<sub>2</sub>, O<sub>2</sub>, CO, and nitrogen (N<sub>2</sub>) are not present in concentrations sufficient to affect the results.

Other methods, as well as modifications to the procedure described herein, are also applicable for some or all of the above determinations. Examples of specific methods and modifications include: (1) a multi-point sampling method using an Orsat analyzer to analyze individual grab samples obtained at each point; (2) a method using CO<sub>2</sub> or O<sub>2</sub> and stoichiometric calculations to determine dry molecular weight and excess air; (3) assigning a value of 30.0 for dry molecular weight, in lieu of actual measurements, for processes burning natural gas, coal, or oil. These methods and modifications may be used, but are subject to the approval of the Administrator.

##### 2. Apparatus

As an alternative to the sampling apparatus and systems described herein, other sampling systems (e.g., liquid displacement) may be used provided such systems are capable of obtaining a representative sample and maintaining a constant sampling rate, and are otherwise capable of yielding acceptable results. Use of such systems is subject to the approval of the Administrator.

###### 2.1 Grab Sampling (Figure 3-1).

2.1.1 Probe. The probe should be made of stainless steel or borosilicate glass tubing and should be equipped with an in-stack or out-stack filter to remove particulate matter (a plug of glass wool is satisfactory for this purpose). Any other material inert to O<sub>2</sub>, CO<sub>2</sub>, CO, and N<sub>2</sub> and resistant to temperature at sampling conditions may be used for the probe; examples of such material are aluminum, copper, quartz glass and Teflon.

2.1.2 Pump. A one-way squeeze bulb, or equivalent, is used to transport the gas sample to the analyzer.

###### 2.2 Integrated Sampling (Figure 3-2).

2.2.1 Probe. A probe such as that described in Section 2.1.1 is suitable.

\* Mention of trade names or specific products does not constitute endorsement by the Environmental Protection Agency.

## RULES AND REGULATIONS

2.2.2 Condenser. An air-cooled or water-cooled condenser, or other condenser that will not remove  $O_2$ ,  $CO_2$ ,  $CO$ , and  $N_2$ , may be used to remove excess moisture which would interfere with the operation of the pump and flow meter.

2.2.3 Valve. A needle valve is used to adjust sample gas flow rate.

2.2.4 Pump. A leak-free, diaphragm-type pump, or equivalent, is used to transport sample gas to the flexible bag. Install a small surge tank between the pump and rate meter to eliminate the pulsation effect of the diaphragm pump on the rotameter.

2.2.5 Rate Meter. The rotameter, or equivalent rate meter, used should be capable of measuring flow rate to within  $\pm 2$  percent of the selected flow rate. A flow rate range of 500 to 1000  $cm^3/min$  is suggested.

2.2.6 Flexible Bag. Any leak-free plastic (e.g., Tedlar, Mylar, Teflon) or plastic-coated aluminum (e.g., aluminized Mylar) bag, or equivalent, having a capacity consistent with the selected flow rate and time length of the test run, may be used. A capacity in the range of 55 to 90 liters is suggested.

To leak-check the bag, connect it to a water manometer and pressurize the bag to 5 to 10 cm  $H_2O$  (2 to 4 in.  $H_2O$ ). Allow to stand for 10 minutes. Any displacement in the water manometer indicates a leak. An alternative leak-check method is to pressurize the bag to 5 to 10 cm  $H_2O$  (2 to 4 in.  $H_2O$ ) and allow to stand overnight. A deflated bag indicates a leak.

2.2.7 Pressure Gauge. A water-filled U-tube manometer, or equivalent, of about 28 cm (12 in.) is used for the flexible bag leak-check.

2.2.8 Vacuum Gauge. A mercury manometer, or equivalent, of at least 760 mm Hg (30 in. Hg) is used for the sampling train leak-check.

2.3 Analysis. For Orsat and Fyrite analyzer maintenance and operation procedures, follow the instructions recommended by the manufacturer, unless otherwise specified herein.

2.3.1 Dry Molecular Weight Determination. An Orsat analyzer or Fyrite type combustion gas analyzer may be used.

2.3.2 Emission Rate Correction Factor or Excess Air Determination. An Orsat analyzer must be used. For low  $CO_2$  (less than 4.0 percent) or high  $O_2$  (greater than 15.0 percent) concentrations, the measuring burette of the Orsat must have at least 0.1 percent subdivisions.

### 3. Dry Molecular Weight Determination

Any of the three sampling and analytical procedures described below may be used for determining the dry molecular weight.

#### 3.1 Single-Point, Grab Sampling and Analytical Procedure.

3.1.1 The sampling point in the duct shall either be at the centroid of the cross section or at a point no closer to the walls than 1.00 m (3.3 ft), unless otherwise specified by the Administrator.

3.1.2 Set up the equipment as shown in Figure 3-1, making sure all connections ahead of the analyzer are tight and leak-free. If an Orsat analyzer is used, it is recommended that the analyzer be leak-checked by following the procedure in Section 5; however, the leak-check is optional.

3.1.3 Place the probe in the stack, with the tip of the probe positioned at the sampling point; purge the sampling line. Draw a sample into the analyzer and immediately analyze it for percent  $CO_2$  and percent  $O_2$ . Determine the percentage of the gas that is  $N_2$  and  $CO$  by subtracting the sum of the percent  $CO_2$  and percent  $O_2$  from 100 percent. Calculate the dry molecular weight as indicated in Section 6.3.

3.1.4 Repeat the sampling, analysis, and calculation procedures, until the dry molecular weights of any three grab samples differ from their mean by no more than 0.3 g/g-mole (0.3 lb/lb-mole). Average these three molecular weights, and report the results to the nearest 0.1 g/g-mole (lb/lb-mole).

#### 3.2 Single-Point, Integrated Sampling and Analytical Procedure.

3.2.1 The sampling point in the duct shall be located as specified in Section 3.1.1.

3.2.2 Leak-check (optional) the flexible bag as in Section 2.2.6. Set up the equipment as shown in Figure 3-2. Just prior to sampling, leak-check (optional) the train by placing a vacuum gauge at the condenser inlet, pulling a vacuum of at least 250 mm Hg (10 in. Hg), plugging the outlet at the quick disconnect, and then turning off the pump. The vacuum should remain stable for at least 0.5 minute. Evacuate the flexible bag. Connect the probe and place it in the stack, with the tip of the probe positioned at the sampling point; purge the sampling line. Next, connect the bag and make sure that all connections are tight and leak free.

3.2.3 Sample at a constant rate. The sampling run should be simultaneous with, and for the same total length of time as, the pollutant emission rate determination. Collection of at least 30 liters (1.00  $ft^3$ ) of sample gas is recommended; however, smaller volumes may be collected, if desired.

3.2.4 Obtain one integrated fine gas sample during each pollutant emission rate determination. Within 8 hours after the sample is taken, analyze it for percent  $CO_2$  and percent  $O_2$  using either an Orsat analyzer or a Fyrite-type combustion gas analyzer. If an Orsat analyzer is used, it is recommended that the Orsat leak-check described in Section 5 be performed before this determination; however, the check is optional. Determine the percentage of the gas that is  $N_2$  and  $CO$  by subtracting the sum of the percent  $CO_2$  and percent  $O_2$

from 100 percent. Calculate the dry molecular weight as indicated in Section 6.3.

3.2.5 Repeat the analysis and calculation procedures until the individual dry molecular weights for any three analyses differ from their mean by no more than 0.3 g/g-mole (0.3 lb/lb-mole). Average these three molecular weights, and report the results to the nearest 0.1 g/g-mole (0.1 lb/lb-mole).

#### 3.3 Multi-Point, Integrated Sampling and Analytical Procedure.

3.3.1 Unless otherwise specified by the Administrator, a minimum of eight traverse points shall be used for circular stacks having diameters less than 0.61 m (24 in.), a minimum of nine shall be used for rectangular stacks having equivalent diameters less than 0.61 m (24 in.), and a minimum of twelve traverse points shall be used for all other cases. The traverse points shall be located according to Method 1. The use of fewer points is subject to approval of the Administrator.

3.3.2 Follow the procedures outlined in Sections 3.2.2 through 3.2.5, except for the following: traverse all sampling points and sample at each point for an equal length of time. Record sampling data as shown in Figure 3-3.

TIME	TRAVERSE PT.	Q 1pm	% DEV. <sup>a</sup>
AVERAGE			

$$^a \% DEV = \left( \frac{Q - Q_{avg}}{Q_{avg}} \right) 100 \quad (\text{MUST BE } \leq 10\%)$$

Figure 3-3. Sampling rate data.

4.1.3 Place the probe in the stack, with the tip of the probe positioned at the sampling point; purge the sampling line. Draw a sample into the analyzer. For emission rate correction factor determination, immediately analyze the sample, as outlined in Sections 4.1.4 and 4.1.5, for percent  $CO_2$  or percent  $O_2$ . If excess air is desired, proceed as follows: (1) immediately analyze the sample, as in Sections 4.1.4 and 4.1.5, for percent  $CO_2$ ,  $O_2$ , and  $CO$ ; (2) determine the percentage of the gas that is  $N_2$  by subtracting the sum of the percent  $CO_2$ , percent  $O_2$ , and percent  $CO$  from 100 percent; and (3) calculate percent excess air as outlined in Section 6.2.

4.1.4 To ensure complete absorption of the  $CO_2$ ,  $O_2$ , or if applicable,  $CO$ , make repeated passes through each absorbing solution until two consecutive readings are the same. Several passes (three or four) should be made between readings. (If constant readings cannot be obtained after three consecutive readings, replace the absorbing solution.)

4.1.5 After the analysis is completed, leak-check (mandatory) the Orsat analyzer once again, as described in Section 5. For the results of the analysis to be valid, the Orsat analyzer must pass this leak test before and after the analysis. **NOTE**—Since this single-point, grab sampling and analytical procedure is normally conducted in conjunction with a single-point, grab sampling and analytical procedure for a pollutant, only one analysis is ordinarily conducted. Therefore, great care must be taken to obtain a valid sample and analysis. Although in most cases only  $CO_2$  or  $O_2$  is required, it is recommended that both  $CO_2$  and  $O_2$  be measured, and that Citation 5 in the Bibliography be used to validate the analytical data.

#### 4.2 Single-Point, Integrated Sampling and Analytical Procedure.

4.2.1 The sampling point in the duct shall be located as specified in Section 4.1.1.

4.2.2 Leak-check (mandatory) the flexible bag as in Section 2.2.6. Set up the equipment as shown in Figure 3-2. Just prior to sampling, leak-check (mandatory) the train by placing a vacuum gauge at the condenser inlet, pulling a vacuum of at least 250 mm Hg (10 in. Hg), plugging the outlet at the quick disconnect, and then

#### 4. Emission Rate Correction Factor or Excess Air Determination

**NOTE**—A Fyrite-type combustion gas analyzer is not acceptable for excess air or emission rate correction factor determination, unless approved by the Administrator. If both percent  $CO_2$  and percent  $O_2$  are measured, the analytical results of any of the three procedures given below may also be used for calculating the dry molecular weight.

Each of the three procedures below shall be used only when specified in an applicable subpart of the standards. The use of these procedures for other purposes must have specific prior approval of the Administrator.

##### 4.1 Single-Point, Grab Sampling and Analytical Procedure.

4.1.1 The sampling point in the duct shall either be at the centroid of the cross-section or at a point no closer to the walls than 1.00 m (3.3 ft), unless otherwise specified by the Administrator.

4.1.2 Set up the equipment as shown in Figure 3-1, making sure all connections ahead of the analyzer are tight and leak-free. Leak-check the Orsat analyzer according to the procedure described in Section 5. This leak-check is mandatory.

turning off the pump. The vacuum shall remain stable for at least 0.5 minute. Evacuate the flexible bag. Connect the probe and place it in the stack, with the tip of the probe positioned at the sampling point; purge the sampling line. Next, connect the bag and make sure that all connections are tight and leak free.

4.2.3 Sample at a constant rate, or as specified by the Administrator. The sampling run must be simultaneous with, and for the same total length of time as, the pollutant emission rate determination. Collect at least 30 liters (1.00  $ft^3$ ) of sample gas. Smaller volumes may be collected, subject to approval of the Administrator.

4.2.4 Obtain one integrated fine gas sample during each pollutant emission rate determination. For emission rate correction factor determination, analyze the sample within 4 hours after it is taken for percent  $CO_2$  or percent  $O_2$  (as outlined in Sections 4.2.5 through 4.2.7). The Orsat analyzer must be leak-checked (see Section 5) before the analysis. If excess air is desired, proceed as follows: (1) within 4 hours after the sample is taken, analyze it (as in Sections 4.2.5 through 4.2.7) for percent  $CO_2$ ,  $O_2$ , and  $CO$ ; (2) determine the percentage of the gas that is  $N_2$  by subtracting the sum of the percent  $CO_2$ , percent  $O_2$ , and percent  $CO$  from 100 percent; (3) calculate percent excess air, as outlined in Section 6.2.

4.2.5 To ensure complete absorption of the  $CO_2$ ,  $O_2$ , or if applicable,  $CO$ , make repeated passes through each absorbing solution until two consecutive readings are the same. Several passes (three or four) should be made between readings. (If constant readings cannot be obtained after three consecutive readings, replace the absorbing solution.)

4.2.6 Repeat the analysis until the following criteria are met:

4.2.6.1 For percent  $CO_2$ , repeat the analytical procedure until the results of any three analyses differ by no more than (a) 0.3 percent by volume when  $CO_2$  is greater than 4.0 percent or (b) 0.2 percent by volume when  $CO_2$  is less than or equal to 4.0 percent. Average the three acceptable values of percent  $CO_2$  and report the results to the nearest 0.1 percent.

4.2.6.2 For percent  $O_2$ , repeat the analytical procedure until the results of any three analyses differ by no more

than (a) 0.3 percent by volume when O<sub>2</sub> is less than 15.0 percent or (b) 0.2 percent by volume when O<sub>2</sub> is greater than 15.0 percent. Average the three acceptable values of percent O<sub>2</sub> and report the results to the nearest 0.1 percent.

4.2.5 For percent CO, repeat the analytical procedure until the results of any three analyses differ by no more than 0.3 percent. Average the three acceptable values of percent CO and report the results to the nearest 0.1 percent.

4.2.7 After the analysis is completed, leak-check (mandatory) the Orsat analyzer once again, as described in Section 5. For the results of the analysis to be valid, the Orsat analyzer must pass this leak test before and after the analysis. Note: Although in most instances only CO<sub>2</sub> or O<sub>2</sub> is required, it is recommended that both CO<sub>2</sub> and O<sub>2</sub> be measured, and that Citation 5 in the Bibliography be used to validate the analytical data.

4.3 Multi-Point, Integrated Sampling and Analytical Procedure.

4.3.1 Both the minimum number of sampling points and the sampling point location shall be as specified in Section 3.1 of this method. The use of fewer points than specified is subject to the approval of the Administrator.

4.3.2 Follow the procedures outlined in Sections 4.2.2 through 4.2.7, except for the following: Traverse all sampling points and sample at each point for an equal length of time. Record sampling data as shown in Figure 3-3.

5. Leak-Check Procedure for Orsat Analyzers

Moving an Orsat analyzer frequently causes it to leak. Therefore, an Orsat analyzer should be thoroughly leak-checked on site before the flue gas sample is introduced into it. The procedure for leak-checking an Orsat analyzer is:

5.1.1 Bring the liquid level in each pipette up to the reference mark on the capillary tubing and then close the pipette stopcock.

5.1.2 Raise the leveling bulb sufficiently to bring the meniscus into the graduated portion of the pipette and then close the manifold stopcock.

5.1.3 Record the meniscus position.

5.1.4 Observe the meniscus in the burette and the liquid level in the pipette for movement over the next 4 minutes.

5.1.5 For the Orsat analyzer to pass the leak-check, two conditions must be met.

5.1.5.1 The liquid level in each pipette must not fall below the bottom of the capillary tubing during this 4-minute interval.

5.1.5.2 The meniscus in the burette must not change by more than 0.2 ml during this 4-minute interval.

5.1.6 If the analyzer fails the leak-check procedure, all rubber connections and stopcocks should be checked until the cause of the leak is identified. Leaking stopcocks must be disassembled, cleaned, and regreased. Leaking rubber connections must be replaced. After the analyzer is reassembled, the leak-check procedure must be repeated.

6. Calculations

6.1 Nomenclature.

- M<sub>d</sub> = Dry molecular weight, g/g-mole (lb/lb-mole).
- %EA = Percent excess air.
- %CO<sub>2</sub> = Percent CO<sub>2</sub> by volume (dry basis).
- %O<sub>2</sub> = Percent O<sub>2</sub> by volume (dry basis).
- %CO = Percent CO by volume (dry basis).
- %N<sub>2</sub> = Percent N<sub>2</sub> by volume (dry basis).
- 0.264 = Ratio of O<sub>2</sub> to N<sub>2</sub> in air, v/v.
- 0.280 = Molecular weight of N<sub>2</sub> or CO, divided by 100.
- 0.320 = Molecular weight of O<sub>2</sub> divided by 100.
- 0.440 = Molecular weight of CO<sub>2</sub> divided by 100.

6.2 Percent Excess Air. Calculate the percent excess air (if applicable), by substituting the appropriate values of percent O<sub>2</sub>, CO, and N<sub>2</sub> (obtained from Section 4.1.3 or 4.2.4) into Equation 3-1.

$$\%EA = \left[ \frac{\%O_2 - 0.5\%CO}{0.264\%N_2 - \%O_2 - 0.5\%CO} \right] 100$$

Equation 3-1

NOTE.—The equation above assumes that ambient air is used as the source of O<sub>2</sub> and that the fuel does not contain appreciable amounts of N<sub>2</sub> (as do coke oven or blast furnace gases). For those cases when appreciable amounts of N<sub>2</sub> are present (coal, oil, and natural gas do not contain appreciable amounts of N<sub>2</sub>) or when oxygen enrichment is used, alternate methods, subject to approval of the Administrator, are required.

6.3 Dry Molecular Weight. Use Equation 3-2 to calculate the dry molecular weight of the stack gas

$$M_d = 0.440(\%CO_2) + 0.320(\%O_2) + 0.280(\%N_2 + \%CO)$$

Equation 3-2

NOTE.—The above equation does not consider argon in air (about 0.9 percent, molecular weight of 39.7). A negative error of about 0.4 percent is introduced. The tester may opt to include argon in the analysis using procedures subject to approval of the Administrator.

7. Bibliography

1. Altshuler, A. P. Storage of Gases and Vapors in Plastic Bags. International Journal of Air and Water Pollution. 6:75-81, 1963.
2. Conner, William D. and J. S. Nader. Air Sampling Plastic Bags. Journal of the American Industrial Hygiene Association. 28:291-297, 1964.
3. Hurrell Manual for Gas Analysts, Seventh edition. Burrell Corporation, 223 Fifth Avenue, Pittsburgh, Pa. 15219, 1951.
4. Mitchell, W. J. and M. R. Mideast. Field Reliability of the Orsat Analyzer. Journal of Air Pollution Control Association 19:491-496, May 1978.
5. Shigehara, R. T., R. M. Neulicht, and W. S. Smith. Validating Orsat Analysis Data from Fossil Fuel-Fired Units. Stack Sampling News. 4(2):21-26, August, 1976.

METHOD 4—DETERMINATION OF MOISTURE CONTENT IN STACK GASES

1. Principle and Applicability

1.1 Principle. A gas sample is extracted at a constant rate from the source; moisture is removed from the sample stream and determined either volumetrically or gravimetrically.

1.2 Applicability. This method is applicable for determining the moisture content of stack gas. Two procedures are given. The first is a reference method, for accurate determinations of moisture content (such as are needed to calculate emission data). The second is an approximation method, which provides estimates of percent moisture to aid in setting isokinetic sampling rates prior to a pollutant emission measurement run. The approximation method described herein is only a suggested approach; alternative means for approximating the moisture content, e.g., drying (tube), wet bulb-dry bulb techniques, condensation techniques, stoichiometric calculations, previous experience, etc., are also acceptable.

The reference method is often conducted simultaneously with a pollutant emission measurement run; when it is, calculation of percent isokinetic pollutant emission rate, etc., for the run shall be based upon the results of the reference method or its equivalent; these calculations shall not be based upon the results of the approximation method, unless the approximation method is shown, to the satisfaction of the Administrator, U.S. Environmental Protection Agency, to be capable of yielding results within 1 percent H<sub>2</sub>O of the reference method.

NOTE.—The reference method may yield questionable results when applied to saturated gas streams or to streams that contain water droplets. Therefore, when these conditions exist or are suspected, a second determination of the moisture content shall be made simultaneously with the reference method, as follows: Assume that the gas stream is saturated. Attach a temperature sensor (capable of measuring to ±1° C (2° F)) to the reference method probe. Measure the stack gas temperature at each traverse point (see Section 2.2.1) during the reference method traverse; calculate the average stack gas temperature. Next, determine the moisture percentage, either by: (1) using a psychrometric chart and making appropriate corrections if stack pressure is different from that of the chart, or (2) using saturation vapor pressure tables. In cases where the psychrometric chart or the saturation vapor pressure tables are not applicable (based on evaluation of the process), alternate methods, subject to the approval of the Administrator, shall be used.

2. Reference Method

The procedure described in Method 5 for determining moisture content is acceptable as a reference method.

2.1 Apparatus. A schematic of the sampling train used in this reference method is shown in Figure 4-1. All components shall be maintained and calibrated according to the procedure outlined in Method 3.

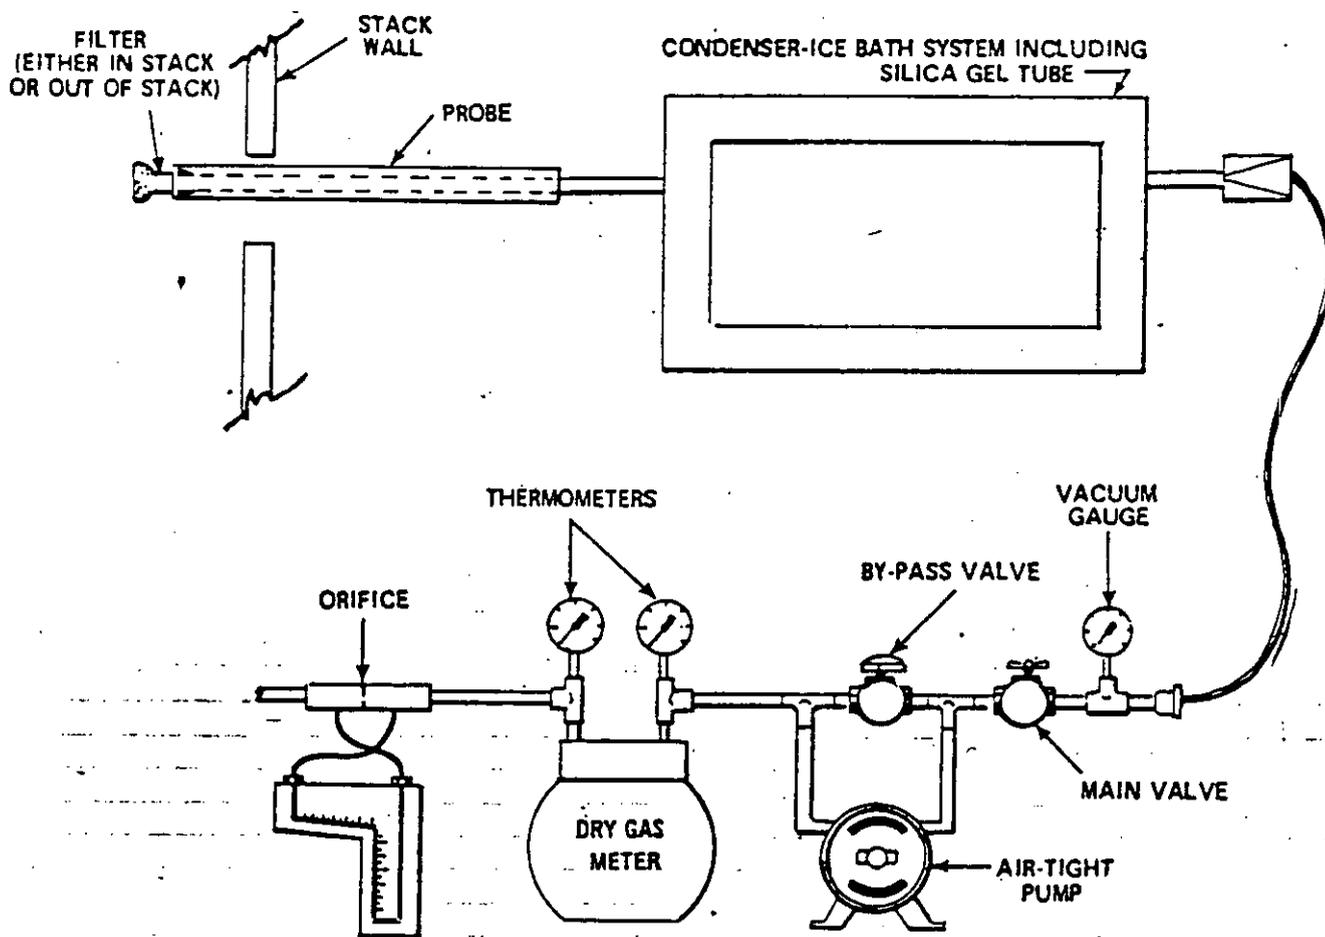


Figure 4-1. Moisture sampling train-reference method.

2.1.1 Probe. The probe is constructed of stainless steel or glass tubing, sufficiently heated to prevent water condensation, and is equipped with a filter, either in-stack (e.g., a plug of glass wool inserted into the end of the probe) or heated out-stack (e.g., as described in Method 5), to remove particulate matter.

When stack conditions permit, other metals or plastic tubing may be used for the probe, subject to the approval of the Administrator.

2.1.2 Condenser. The condenser consists of four impingers connected in series with ground glass, leak-free fittings or any similarly leak-free non-contaminating fittings. The first, third, and fourth impingers shall be of the Greenburg-Smith design, modified by replacing the tip with a 1.3 centimeter ( $\frac{1}{2}$  inch) LD glass tube extending to about 1.3 cm ( $\frac{1}{2}$  in.) from the bottom of the flask. The second impinger shall be of the Greenburg-Smith design with the standard tip. Modifications (e.g., using flexible connections between the impingers, using materials other than glass, or using flexible vacuum lines to connect the filter holder to the condenser) may be used, subject to the approval of the Administrator.

The first two impingers shall contain known volumes of water, the third shall be empty, and the fourth shall contain a known weight of 6- to 16-mesh indicating type silica gel, or equivalent desiccant. If the silica gel has been previously used, dry at 175° C (350° F) for 2 hours. New silica gel may be used as received. A thermometer, capable of measuring temperature to within 1° C (2° F), shall be placed at the outlet of the fourth impinger, for monitoring purposes.

Alternatively, any system may be used (subject to the approval of the Administrator) that cools the sample gas stream and allows measurement of both the water that has been condensed and the moisture leaving the condenser, each to within 1 ml or 1 g. Acceptable means are to measure the condensed water, either gravimetrically or volumetrically, and to measure the moisture leaving the condenser by: (1) monitoring the temperature and pressure at the exit of the condenser and using Dalton's law of partial pressures, or (2) passing

the sample gas stream through a tared silica gel (or equivalent desiccant) trap, with exit gases kept below 20° C (68° F), and determining the weight gain.

If means other than silica gel are used to determine the amount of moisture leaving the condenser, it is recommended that silica gel (or equivalent) still be used between the condenser system and pump, to prevent moisture condensation in the pump and metering devices and to avoid the need to make corrections for moisture in the metered volume.

2.1.3 Cooling System. An ice bath container and crushed ice (or equivalent) are used to aid in condensing moisture.

2.1.4 Metering System. This system includes a vacuum gauge, leak-free pump, thermometers capable of measuring temperature to within 3° C (5.4° F), dry gas meter capable of measuring volume to within 2 percent, and related equipment as shown in Figure 4-1. Other metering systems, capable of maintaining a constant sampling rate and determining sample gas volume, may be used, subject to the approval of the Administrator.

2.1.5 Barometer, Mercury, aneroid, or other barometer capable of measuring atmospheric pressure to within 2.5 mm Hg (0.1 in. Hg) may be used. In many cases, the barometric reading may be obtained from a nearby national weather service station, in which case the station value (which is the absolute barometric pressure) shall be requested and an adjustment for elevation differences between the weather station and the sampling point shall be applied at a rate of minus 2.5 mm Hg (0.1 in. Hg) per 30 m (100 ft) elevation increase or vice versa for elevation decrease.

2.1.6 Graduated Cylinder and/or Balance. These items are used to measure condensed water and moisture caught in the silica gel to within 1 ml or 0.5 g. Graduated cylinders shall have subdivisions no greater than 2 ml. Most laboratory balances are capable of weighing to the nearest 0.5 g or less. These balances are suitable for use here.

2.2 Procedure. The following procedure is written for a condenser system (such as the impinger system de-

scribed in Section 2.1.2) incorporating volumetric analysis to measure the condensed moisture, and silica gel and gravimetric analysis to measure the moisture leaving the condenser.

2.2.1 Unless otherwise specified by the Administrator, a minimum of eight traverse points shall be used for circular stacks having diameters less than 0.61 m (24 in.), a minimum of nine points shall be used for rectangular stacks having equivalent diameters less than 0.61 m (24 in.), and a minimum of twelve traverse points shall be used in all other cases. The traverse points shall be located according to Method 1. The use of fewer points is subject to the approval of the Administrator. Select a suitable probe and probe length such that all traverse points can be sampled. Consider sampling from opposite sides of the stack (four total sampling ports) for large stacks, to permit use of shorter probe lengths. Mark the probe with heat resistant tape or by some other method to denote the proper distance into the stack or duct for each sampling point. Place known volumes of water in the first two impingers. Weigh and record the weight of the silica gel to the nearest 0.5 g, and transfer the silica gel to the fourth impinger; alternatively, the silica gel may first be transferred to the impinger, and the weight of the silica gel plus impinger recorded.

2.2.2 Select a total sampling time such that a minimum total gas volume of 0.50 scm (21 acf) will be collected, at a rate no greater than 0.021 m<sup>3</sup>/min (0.75 cfm). When both moisture content and pollutant emission rate are to be determined, the moisture determination shall be simultaneous with, and for the same total length of time as, the pollutant emission rate run, unless otherwise specified in an applicable subpart of the standards.

2.2.3 Set up the sampling train as shown in Figure 4-1. Turn on the probe heater and (if applicable) the filter heating system to temperatures of about 120° C (248° F), to prevent water condensation ahead of the condenser; allow time for the temperatures to stabilize. Place crushed ice in the ice bath container. It is recommended, but not required, that a leak check be done, as follows: Disconnect the probe from the first impinger or



	IMPINGER VOLUME, ml	SILICA GEL WEIGHT, g
FINAL		
INITIAL		
DIFFERENCE		

Figure 4-1. Analytical data—reference method.

## 2.3.1 Nomenclature.

- $B_{ws}$  = Proportion of water vapor, by volume, in the gas stream.  
 $M_w$  = Molecular weight of water, 18.0 (lb-mole) (18.0152 g-mole).  
 $P_m$  = Absolute pressure (for this method, same as barometric pressure) at the dry gas meter, mm Hg (in. Hg).  
 $P_{std}$  = Standard absolute pressure, 760 mm Hg (29.92 in. Hg).  
 $R$  = Ideal gas constant, 0.08206 (mm Hg) (m<sup>3</sup>)/(g-mole) (°K) (or metric units and 21.85 (in. Hg) (ft<sup>3</sup>)/(lb-mole) (°R) for English units.  
 $T_m$  = Absolute temperature at meter, °K (°R).  
 $T_{std}$  = Standard absolute temperature, 293° K (625° R).  
 $V_m$  = Dry gas volume measured by dry gas meter, dcm (dcft).  
 $\Delta V_m$  = Incremental dry gas volume measured by dry gas meter at each traverse point, dcm (dcft).  
 $V_{m(std)}$  = Dry gas volume measured by the dry gas meter, corrected to standard conditions, dcm (dcft).  
 $V_{w(std)}$  = Volume of water vapor condensed corrected to standard conditions, scm (scf).  
 $V_{ws(std)}$  = Volume of water vapor collected in silica gel corrected to standard conditions, scm (scf).  
 $V_f$  = Final volume of condenser water, ml.  
 $V_i$  = Initial volume, if any, of condenser water, ml.  
 $W_f$  = Final weight of silica gel or silica gel plus impinger, g.  
 $W_i$  = Initial weight of silica gel or silica gel plus impinger, g.  
 $Y$  = Dry gas meter calibration factor.  
 $\rho_w$  = Density of water, 0.9982 g/ml (0.002201 lb/ml).

## 2.3.2 Volume of water vapor condensed.

$$V_{w(std)} = \frac{(V_f - V_i) \rho_w R T_{std}}{P_{std} M_w} = K_1 (V_f - V_i)$$

Equation 4-1

where:

- $K_1 = 0.001333$  m<sup>3</sup>/ml for metric units  
 $= 0.04707$  ft<sup>3</sup>/ml for English units

## 2.3.3 Volume of water vapor collected in silica gel.

$$V_{ws(std)} = \frac{(W_f - W_i) R T_{std}}{P_{std} M_w} = K_2 (W_f - W_i)$$

Equation 4-2

where:

- $K_2 = 0.001335$  m<sup>3</sup>/g for metric units  
 $= 0.04718$  ft<sup>3</sup>/g for English units

## 2.3.4 Sample gas volume.

$$V_{m(std)} = V_m Y \frac{(P_m)(T_{std})}{(P_{std})(T_m)} = K_3 Y \frac{V_m P_m}{T_m}$$

Equation 4-3

where:

- $K_3 = 0.3508$  °K/mm Hg for metric units  
 $= 17.64$  °R/in. Hg for English units

NOTE.—If the post-test leak rate (Section 2.2.6) exceeds the allowable rate, correct the value of  $V_m$  in Equation 4-3, as described in Section 6.3 of Method 3.

## 2.3.5 Moisture Content.

$$B_{ws} = \frac{V_{w(std)} + V_{ws(std)}}{V_{m(std)} + V_{w(std)} + V_{ws(std)} + V_m(std)}$$

Equation 4-4

NOTE.—In saturated or moisture droplet-laden gas streams, two calculations of the moisture content of the stack gas shall be made, one using a value based upon the saturated conditions (see Section 1.2), and another based upon the results of the impinger analysis. The lower of these two values of  $B_{ws}$  shall be considered correct.

2.3.6 Verification of constant sampling rate. For each time increment, determine the  $\Delta V_m$ . Calculate the average. If the value for any time increment differs from the average by more than 10 percent, reject the results and repeat the run.

## 3. Approximation Method

The approximation method described below is presented only as a suggested method (see Section 1.2).

## 3.1 Apparatus.

3.1.1 Probe. Stainless steel or glass tubing, sufficiently heated to prevent water condensation and equipped with a filter (either in-stack or heated out-stack) to remove particulate matter. A ping of glass wool, inserted into the end of the probe, is a satisfactory filter.

3.1.2 Impingers. Two midjet impingers, each with 30 ml capacity, or equivalent.

3.1.3 Ice Bath. Container and ice, to aid in condensing moisture in impingers.

3.1.4 Drying Tube. Tube packed with new or regenerated 6- to 16-mesh indicating-type silica gel (or equivalent desiccant), to dry the sample gas and to protect the meter and pump.

3.1.5 Valve. Needle valve, to regulate the sample gas flow rate.

3.1.6 Pump. Leak-free, diaphragm type, or equivalent, to pull the gas sample through the train.

3.1.7 Volume meter. Dry gas meter, sufficiently accurate to measure the sample volume within 2%, and calibrated over the range of flow rates and conditions actually encountered during sampling.

3.1.8 Rate Meter. Rotameter, to measure the flow rate from 0 to 3 lpm (0 to 0.11 cfm).

3.1.9 Graduated Cylinder. 25 ml.

3.1.10 Barometer. Mercury, aneroid, or other barometer, as described in Section 2.1.5 above.

3.1.11 Vacuum Gauge. At least 750 mm Hg (30 in. Hg) gauge, to be used for the sampling leak check.

## 3.2 Procedure.

3.2.1 Place exactly 5 ml distilled water in each impinger. Assemble the apparatus without the probe as shown in Figure 4-4. Leak check the train by placing a vacuum gauge at the inlet to the first impinger and drawing a vacuum of at least 250 mm Hg (10 in. Hg), plugging the outlet of the rotameter, and then turning off the pump. The vacuum shall remain constant for at least one minute. Carefully release the vacuum gauge before unplugging the rotameter end.

## RULES AND REGULATIONS

3.2.2 Connect the probe, insert it into the stack, and sample at a constant rate of 2 lpm (0.071 cfm). Continue sampling until the dry gas meter registers about 30 liters (1.1 ft<sup>3</sup>) or until visible liquid droplets are carried over from the first impinger to the second. Record temperature, pressure, and dry gas meter readings as required by Figure 4-3.

3.2.3 After collecting the sample, combine the contents of the two impingers and measure the volume to the nearest 0.5 ml.

3.3 Calculations. The calculation method presented is designed to estimate the moisture in the stack gas; therefore, other data, which are only necessary for accurate moisture determinations, are not collected. The following equations adequately estimate the moisture content, for the purpose of determining isokinetic sampling rate settings.

## 3.3.1 Nomenclature.

- $B_{ws}$  = Approximate proportion, by volume, of water vapor in the gas stream leaving the second impinger, 0.025.  
 $B_{wv}$  = Water vapor in the gas stream, proportion by volume.  
 $M_w$  = Molecular weight of water, 18.0 g/g-mole (18.0 lb/lb-mole)  
 $P_m$  = Absolute pressure (for this method, same as barometric pressure) at the dry gas meter.  
 $P_{std}$  = Standard absolute pressure, 760 mm Hg (29.92 in. Hg).  
 $R$  = Ideal gas constant, 0.08206 (mm Hg) (m<sup>3</sup>) / (g-mole) (°K) for metric units and 21.85 (in. Hg) (ft<sup>3</sup>) / (lb-mole) (°R) for English units.  
 $T_m$  = Absolute temperature at meter, °K (°R)  
 $T_{std}$  = Standard absolute temperature, 293° K (528° R)  
 $V_f$  = Final volume of impinger contents, ml.  
 $V_i$  = Initial volume of impinger contents, ml.  
 $V_m$  = Dry gas volume measured by dry gas meter, decm (dscf).  
 $V_{m(Std)}$  = Dry gas volume measured by dry gas meter, corrected to standard conditions, decm (dscf).  
 $V_{w(Std)}$  = Volume of water vapor condensed, corrected to standard conditions, scm (scf).  
 $\rho_w$  = Density of water, 0.9982 g/ml (0.002201 lb/ml).

## 3.3.2 Volume of water vapor collected.

$$V_{wv} = \frac{(V_f - V_i) \rho_w RT_{std}}{P_m M_w} \\ = K_1 (V_f - V_i)$$

Equation 4-5

where:

- $K_1 = 0.001333$  m<sup>3</sup>/ml for metric units  
 $= 0.04707$  ft<sup>3</sup>/ml for English units.

## 3.3.3 Gas volume.

$$V_{m(Std)} = V_m \left( \frac{P_m}{P_{std}} \right) \left( \frac{T_{std}}{T_m} \right) \\ = K_2 \frac{V_m P_m}{T_m}$$

Equation 4-6

where:

- $K_2 = 0.3856$  °K/mm Hg for metric units  
 $= 17.04$  °R/in. Hg for English units

## 3.3.4 Approximate moisture content.

$$B_{ws} = \frac{V_{wv}}{V_{wv} + V_{m(Std)}} + B_{wv} \\ = \frac{V_{wv}}{V_{wv} + V_{m(Std)}} + (0.025)$$

Equation 4-7

## 4. Calibration

4.1 For the reference method, calibrate equipment as specified in the following sections of Method 5: Section 5.3 (metering system); Section 5.5 (temperature gauges); and Section 5.7 (barometer). The recommended leak check of the metering system (Section 5.6 of Method 5) also applies to the reference method. For the approximation method, use the procedures outlined in Section 5.1.1 of Method 6 to calibrate the metering system, and the procedure of Method 5, Section 5.7 to calibrate the barometer.

## 5. Bibliography

1. Air Pollution Engineering Manual (Second Edition), Danielson, J. A. (ed.), U.S. Environmental Protection Agency, Office of Air Quality Planning and Standards, Research Triangle Park, N.C. Publication No. AP-40, 1973.
2. Devorkin, Howard, et al. Air Pollution Source Testing Manual, Air Pollution Control District, Los Angeles, Calif. November, 1963.
3. Methods for Determination of Velocity, Volume, Dust and Mist Content of Gases, Western Precipitation Division of Joy Manufacturing Co., Los Angeles, Calif. Bulletin WP-50, 1968.

## METHOD 5—DETERMINATION OF PARTICULATE EMISSIONS FROM STATIONARY SOURCES

## 1. Principle and Applicability

1.1 Principle. Particulate matter is withdrawn isokinetically from the source and collected on a glass fiber filter maintained at a temperature in the range of 120±14° C (248±25° F) or such other temperature as specified by an applicable subpart of the standards or approved by the Administrator, U.S. Environmental Protection Agency, for a particular application. The particulate mass, which includes any material that condenses at or above the filtration temperature, is determined gravimetrically after removal of uncombined water.

1.2 Applicability. This method is applicable for the determination of particulate emissions from stationary sources.

## 2. Apparatus

2.1 Sampling Train. A schematic of the sampling train used in this method is shown in Figure 5-1. Complete construction details are given in APTD-0581 (Citation 2 in Section 7); commercial models of this train are also available. For changes from APTD-0581 and for allowable modifications of the train shown in Figure 5-1, see the following subsections.

The operating and maintenance procedures for the sampling train are described in APTD-0576 (Citation 3 in Section 7). Since correct usage is important in obtaining valid results, all users should read APTD-0576 and adopt the operating and maintenance procedures outlined in it, unless otherwise specified herein. The sampling train consists of the following components:

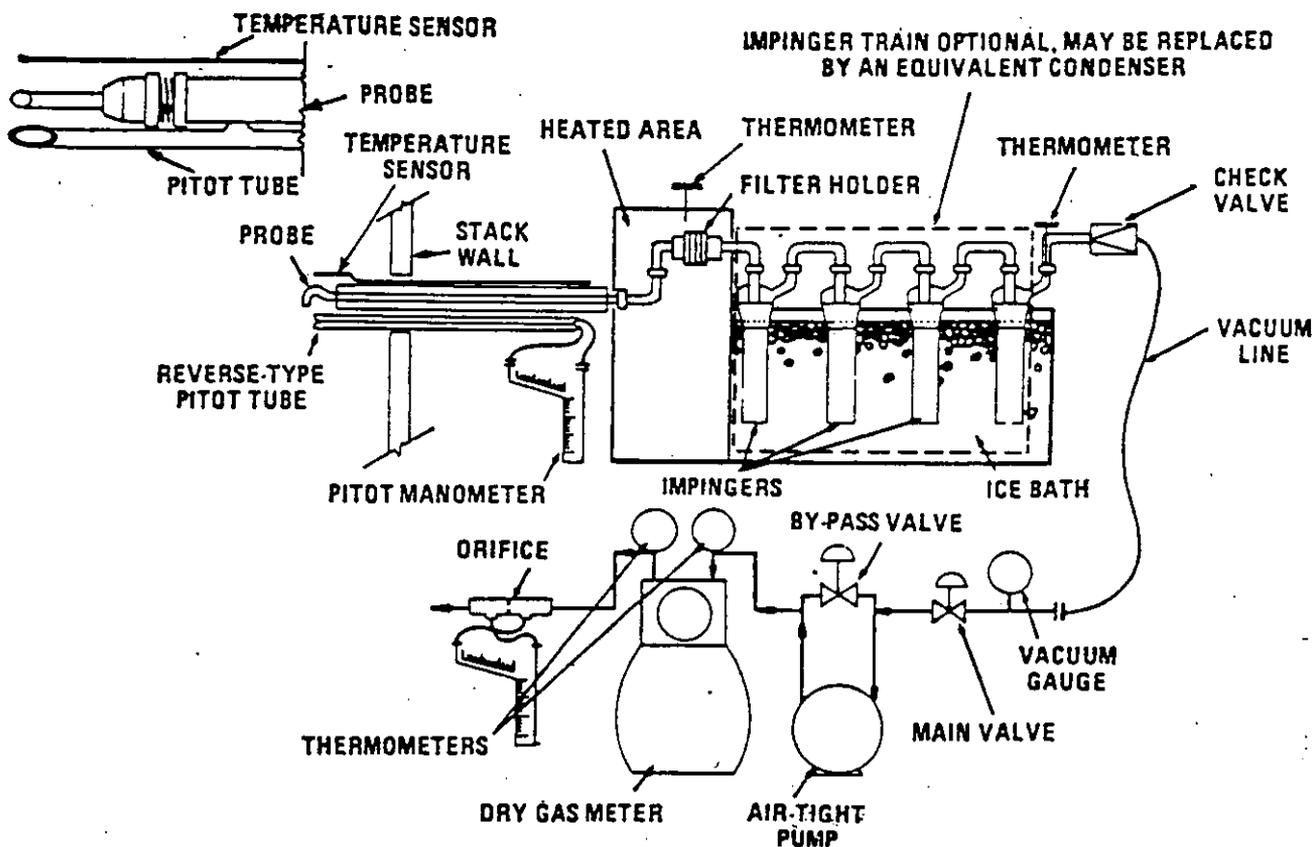


Figure 5-1. Particulate-sampling train.

2.1.1 Probe Nozzle. Stainless steel (316) or glass with sharp, tapered leading edge. The angle of taper shall be  $\leq 30^\circ$  and the taper shall be on the outside to preserve a constant internal diameter. The probe nozzle shall be of the button-hook or elbow design, unless otherwise specified by the Administrator. If made of stainless steel, the nozzle shall be constructed from seamless tubing; other materials of construction may be used, subject to the approval of the Administrator.

A range of nozzle sizes suitable for isokinetic sampling should be available, e.g., 0.32 to 1.27 cm ( $1/8$  to  $1/2$  in.)—or larger if higher volume sampling trains are used—inside diameter (ID) nozzles in increments of 0.16 cm ( $1/16$  in.). Each nozzle shall be calibrated according to the procedures outlined in Section 5.

2.1.2 Probe Liner. Borosilicate or quartz glass tubing with a heating system capable of maintaining a gas temperature at the exit and during sampling of  $120 \pm 14^\circ\text{C}$  ( $248 \pm 25^\circ\text{F}$ ), or such other temperature as specified by an applicable subpart of the standards or approved by the Administrator for a particular application. (The tester may opt to operate the equipment at a temperature lower than that specified.) Since the actual temperature at the outlet of the probe is not usually monitored during sampling, probes constructed according to APTD-0581 and utilizing the calibration curves of APTD-0576 (or calibrated according to the procedure outlined in APTD-0576) will be considered acceptable.

Either borosilicate or quartz glass probe liners may be used for stack temperatures up to about  $450^\circ\text{C}$  ( $900^\circ\text{F}$ ); quartz liners shall be used for temperatures between 480 and  $900^\circ\text{C}$  ( $900$  and  $1,650^\circ\text{F}$ ). Both types of liners may be used at higher temperatures than specified for short periods of time, subject to the approval of the Administrator. The softening temperature for borosilicate is  $820^\circ\text{C}$  ( $1,508^\circ\text{F}$ ), and for quartz it is  $1,504^\circ\text{C}$  ( $2,732^\circ\text{F}$ ).

Whenever practical, every effort should be made to use borosilicate or quartz glass probe liners. Alternatively, metal liners (e.g., 316 stainless steel, Inconel 825, or other corrosion resistant metals) made of seamless tubing may be used, subject to the approval of the Administrator.

2.1.3 Pitot Tube, Type S, as described in Section 2.1 of Method 2, or other device approved by the Administrator. The pitot tube shall be attached to the probe (as shown in Figure 5-1) to allow constant monitoring of the stack gas velocity. The impact (high pressure) opening

plane of the pitot tube shall be even with or above the nozzle entry plane (see Method 2, Figure 2-6b) during sampling. The Type S pitot tube assembly shall have a known coefficient, determined as outlined in Section 4 of Method 2.

2.1.4 Differentia. Pressure Gauge. Inclined manometer or equivalent device (two), as described in Section 2.2 of Method 2. One manometer shall be used of velocity head ( $\Delta p$ ) readings, and the other, or orifice differentia, pressure readings.

2.1.5 Filter Holder. Borosilicate glass, with a glass frit filter support and a silicone rubber gasket. Other materials of construction (e.g., stainless steel, Teflon, Viton) may be used, subject to approval of the Administrator. The holder design shall provide a positive seal against leakage from the outside or around the filter. The holder shall be attached immediately at the outlet of the probe (or cyclone, if used).

2.1.6 Filter Heating System. Any heating system capable of maintaining a temperature around the filter holder during sampling of  $120 \pm 14^\circ\text{C}$  ( $248 \pm 25^\circ\text{F}$ ), or such other temperature as specified by an applicable subpart of the standards or approved by the Administrator for a particular application. Alternatively, the tester may opt to operate the equipment at a temperature lower than that specified. A temperature gauge capable of measuring temperature to within  $3^\circ\text{C}$  ( $5.4^\circ\text{F}$ ) shall be installed so that the temperature around the filter holder can be regulated and monitored during sampling. Heating systems other than the one shown in APTD-0581 may be used.

2.1.7 Condenser. The following system shall be used to determine the stack gas moisture content: Four impingers connected in series with leak-free ground glass fittings or any similar leak-free non-contaminating fittings. The first, third, and fourth impingers shall be of the Greenburg-Smith design, modified by replacing the tip with 1.3 cm ( $1/2$  in.) ID glass tube extending to about 1.3 cm ( $1/2$  in.) from the bottom of the flask. The second impinger shall be of the Greenburg-Smith design with the standard tip. Modifications (e.g., using flexible connections between the impingers, using materials other than glass, or using flexible vacuum lines to connect the filter holder to the condenser) may be used, subject to the approval of the Administrator. The first and second impingers shall contain known quantities of water (Section 4.1.3), the third shall be empty, and the fourth shall contain a known weight of silica gel, or equivalent desiccant. A thermometer, capable of measur-

ing temperature to within  $1^\circ\text{C}$  ( $2^\circ\text{F}$ ) shall be placed at the outlet of the fourth impinger for monitoring purposes.

Alternatively, any system that cools the sample gas stream and allows measurement of the water condensed and moisture leaving the condenser, each to within 1 ml or 1 g may be used, subject to the approval of the Administrator. Acceptable means are to measure the condensed water either gravimetrically or volumetrically and to measure the moisture leaving the condenser by: (1) monitoring the temperature and pressure at the exit of the condenser and using Dalton's law of partial pressures; or (2) passing the sample gas stream through a tared silica gel (or equivalent desiccant) trap with exit gases kept below  $20^\circ\text{C}$  ( $68^\circ\text{F}$ ) and determining the weight gain.

If means other than silica gel are used to determine the amount of moisture leaving the condenser, it is recommended that silica gel (or equivalent) still be used between the condenser system and pump to prevent moisture condensation in the pump and metering devices and to avoid the need to make corrections for moisture in the metered volume.

Note.—If a determination of the particulate matter collected in the impingers is desired in addition to moisture content, the impinger system described above shall be used, without modification. Individuals, States or control agencies requiring this information shall be contacted as to the sample recovery and analysis of the impinger contents.

2.1.8 Metering System. Vacuum gauge, leak-free pump, thermometers capable of measuring temperature to within  $3^\circ\text{C}$  ( $5.4^\circ\text{F}$ ), dry gas meter capable of measuring volume to within 2 percent, and related equipment, as shown in Figure 5-1. Other metering systems capable of maintaining sampling rates within 10 percent of isokinetic and of determining sample volume to within 2 percent may be used, subject to the approval of the Administrator. When the metering system is used in conjunction with a pitot tube, the system shall enable checks of isokinetic rates.

Sampling trains utilizing metering systems designed for higher flow rates than that described in APTD-0581 or APTD-0576 may be used provided that the specifications of this method are met.

2.1.9 Barometer. Mercury, aneroid, or other barometer capable of measuring atmospheric pressure to within 2.5 mm Hg (0.1 in. Hg). In many cases, the barometric reading may be obtained from a nearby national weather service station, in which case the station value (which is

1 Mention of trade names or specific products does not constitute endorsement by the Environmental Protection Agency.

22

the absolute barometric pressure) shall be requested and an adjustment for elevation difference between the weather station and sampling point shall be applied at a rate of minus 2.5 mm Hg (0.1 in. Hg) per 30 m (100 ft) elevation increase or vice versa for elevation decrease.

**2.1.10 Gas Density Determination Equipment.** Temperature sensor and pressure gauge, as described in Sections 2.3 and 2.4 of Method 2, and gas analyzer, if necessary, as described in Method 3. The temperature sensor shall, preferably, be permanently attached to the pitot tube or sampling probe in a fixed configuration, such that the tip of the sensor extends beyond the leading edge of the probe sheath and does not touch any metal. Alternatively, the sensor may be attached just prior to use in the field. Note, however, that if the temperature sensor is attached in the field, the sensor must be placed in an interference-free arrangement with respect to the Type S pitot tube openings (see Method 2, Figure 2-7). As a second alternative, if a difference of not more than 1 percent in the average velocity measurement is to be introduced, the temperature gauge need not be attached to the probe or pitot tube. (This alternative is subject to the approval of the Administrator.)

**2.2 Sample Recovery.** The following items are needed:

**2.2.1 Probe-Liner and Probe-Nozzle Brushes.** Nylon bristle brushes with stainless steel wire handles. The probe brush shall have extensions (at least as long as the probe) of stainless steel, Nylon, Teflon, or similarly inert material. The brushes shall be properly sized and shaped to brush out the probe liner and nozzle.

**2.2.2 Wash Bottles—Two.** Glass wash bottles are recommended; polyethylene wash bottles may be used at the option of the tester. It is recommended that acetone not be stored in polyethylene bottles for longer than a month.

**2.2.3 Glass Sample Storage Containers.** Chemically resistant, borosilicate glass bottles, for acetone washes, 500 ml or 1000 ml. Screw cap liners shall either be rubber-gasketed Teflon or shall be constructed so as to be leak-free and resistant to chemical attack by acetone. (Narrow mouth glass bottles have been found to be less prone to leakage.) Alternatively, polyethylene bottles may be used.

**2.2.4 Petri Dishes.** For filter samples, glass or polyethylene, unless otherwise specified by the Administrator.

**2.2.5 Graduated Cylinder and/or Balance.** To measure condensed water to within 1 ml or 1 g. Graduated cylinders shall have subdivisions no greater than 2 ml. Most laboratory balances are capable of weighing to the nearest 0.5 g or less. Any of these balances is suitable for use here and in Section 2.3.4.

**2.2.6 Plastic Storage Containers.** Air-tight containers to store silica gel.

**2.2.7 Funnel and Rubber Policeman.** To aid in transfer of silica gel to container; not necessary if silica gel is weighed in the field.

**2.2.8 Funnel.** Glass or polyethylene, to aid in sample recovery.

**2.3 Analysis.** For analysis, the following equipment is needed.

**2.3.1 Glass Weighing Dishes.**

**2.3.2 Desiccator.**

**2.3.3 Analytical Balance.** To measure to within 0.1 mg.

**2.3.4 Balance.** To measure to within 0.5 g.

**2.3.5 Beakers.** 250 ml.

**2.3.6 Hygrometer.** To measure the relative humidity of the laboratory environment.

**2.3.7 Temperature Gauge.** To measure the temperature of the laboratory environment.

### 3. Reagents

**3.1 Sampling.** The reagents used in sampling are as follows:

**3.1.1 Filters.** Glass fiber filters, without organic binder, exhibiting at least 99.95 percent efficiency ( $\leq 0.05$  percent penetration) on 0.3-micron dioctyl phthalate smoke particles. The filter efficiency test shall be conducted in accordance with ASTM standard method D 2066-71. Test data from the supplier's quality control program are sufficient for this purpose.

**3.1.2 Silica Gel.** Indicating type, 6 to 16 mesh, if previously used, dry at 175° C (350° F) for 2 hours. New silica gel may be used as received. Alternatively, other types of desiccants (equivalent or better) may be used, subject to the approval of the Administrator.

**3.1.3 Water.** When analysis of the material caught in the impingers is required, distilled water shall be used. Run blanks prior to field use to eliminate a high blank on test samples.

**3.1.4 Crushed Ice.**

**3.1.5 Stopcock Grease.** Acetone-insoluble, heat-stable silicone grease. This is not necessary if screw-on connectors with Teflon sleeves, or similar, are used. Alternatively, other types of stopcock grease may be used, subject to the approval of the Administrator.

**3.2 Sample Recovery.** Acetone—reagent grade,  $\leq 0.001$  percent residue, in glass bottles—is required. Acetone from metal containers generally has a high residue blank and should not be used. Sometimes, suppliers transfer acetone to glass bottles from metal containers; thus, acetone blanks shall be run prior to field use and only acetone with low blank values ( $\leq 0.001$  percent) shall be used. In no case shall a blank value of greater than 0.001 percent of the weight of acetone used be subtracted from the sample weight.

**3.3 Analysis.** Two reagents are required for the analysis:

**3.3.1 Acetone.** Same as 3.2.

**3.3.2 Desiccant.** Anhydrous calcium sulfate, indicating type. Subject to the approval of the Administrator.

### 4. Procedure

**4.1 Sampling.** The complexity of this method is such that, in order to obtain reliable results, testers should be trained and experienced with the test procedures.

**4.1.1 Pretest Preparation.** All the components shall be maintained and calibrated according to the procedure described in APTD-0576, unless otherwise specified herein.

Weigh several 200 to 300 g portions of silica gel in air-tight containers to the nearest 0.5 g. Record the total weight of the silica gel plus container, on each container. As an alternative, the silica gel need not be preweighed, but may be weighed directly in its impinger or sampling holder just prior to train assembly.

Check filters visually against light for irregularities and flaws or pinhole leaks. Label filters of the proper diameter on the back side near the edge using numbering machine ink. As an alternative, label the shipping containers (glass or plastic petri dishes) and keep the filters in these containers at all times except during sampling and weighing.

Desiccate the filters at 20 $\pm$ 5.6° C (68 $\pm$ 10° F) and ambient pressure for at least 24 hours and weight at intervals of at least 4 hours to a constant weight, i.e.,  $<0.5$  mg change from previous weighing; record results to the nearest 0.1 mg. During each weighing the filter must not be exposed to the laboratory atmosphere for a period greater than 2 minutes and a relative humidity above 50 percent. Alternatively (unless otherwise specified by the Administrator), the filters may be oven dried at 105° C (220° F) for 2 to 3 hours, desiccated for 2 hours, and weighed. Procedures other than those described, which account for relative humidity effects, may be used, subject to the approval of the Administrator.

**4.1.2 Preliminary Determinations.** Select the sampling site and the minimum number of sampling points according to Method 1 or as specified by the Administrator. Determine the stack pressure, temperature, and the range of velocity heads using Method 2; it is recommended that a leak-check of the pitot lines (see Method 2, Section 4.1) be performed. Determine the moisture content using Approximation Method 4 or its alternatives for the purposes of making isokinetic sampling rate settings. Determine the stack gas dry molecular weight, as described in Method 2, Section 3.5; if integrated Method 3 sampling is used for molecular weight determination, the integrated bag sample shall be taken simultaneously with, and for the same total length of time as, the particulate sample run.

Select a nozzle size based on the range of velocity heads, such that it is not necessary to change the nozzle size in order to maintain isokinetic sampling rates. During the run, do not change the nozzle size. Ensure that the proper differential pressure gauge is chosen for the range of velocity heads encountered (see Section 2.2 of Method 2).

Select a suitable probe liner and probe length such that all traverse points can be sampled. For large stacks, consider sampling from opposite sides of the stack to reduce the length of probes.

Select a total sampling time greater than or equal to the minimum total sampling time specified in the test procedures for the specific industry such that (1) the sampling time per point is not less than 2 min (or some greater time interval as specified by the Administrator), and (2) the sample volume taken (corrected to standard conditions) will exceed the required minimum total gas sample volume. The latter is based on an approximate average sampling rate.

It is recommended that the number of minutes sampled at each point be an integer or an integer plus one-half minute. In order to avoid timing errors.

In some circumstances, e.g., batch cycles, it may be necessary to sample for shorter times at the traverse points and to obtain smaller gas sample volumes. In these cases, the Administrator's approval must first be obtained.

**4.1.3 Preparation of Collection Train.** During preparation and assembly of the sampling train, keep all openings where contamination can occur covered until just prior to assembly or until sampling is about to begin.

Place 100 ml of water in each of the first two impingers. Leave the third impinger empty, and transfer approximately 200 to 300 g of preweighed silica gel from its container to the fourth impinger. Moisten silica gel may be used, but care should be taken to ensure that it is not entrained and carried out from the impinger during sampling. Place the container in a clean place for later use in the sample recovery. Alternatively, the weight of the silica gel plus impinger may be determined to the nearest 0.5 g and recorded.

Using a tweezer or clean disposable surgical gloves, place a labeled (identified) and weighed filter in the filter holder. Be sure that the filter is properly centered and the gasket properly placed so as to prevent the sample gas stream from circumventing the filter. Check the filter for tears after assembly is completed.

When glass liners are used, install the selected nozzle using a Viton A O-ring when stack temperatures are less than 250° C (500° F) and an asbestos string gasket when temperatures are higher. See APTD-0576 for

details. Other connecting systems using either 316 stainless steel or Teflon ferrules may be used. When metal liners are used, install the nozzle as above or by a leak-free direct mechanical connection. Mark the probe with heat resistant tape or by some other method to denote the proper distance into the stack or duct for each sampling point.

Set up the train as in Figure 5-1, using (if necessary) a very light coat of silicone grease on all ground glass joints, greasing only the outer portion (see APTD-0576) to avoid possibility of contamination by the silicone grease. Subject to the approval of the Administrator, a glass cyclone may be used between the probe and filter holder when the total particulate catch is expected to exceed 100 mg or when water droplets are present in the stack gas.

Place crushed ice around the impingers.

**4.1.4 Leak-Check Procedures.**

**4.1.4.1 Pretest Leak-Check.** A pretest leak-check is recommended, but not required. If the tester opts to conduct the pretest leak-check, the following procedure shall be used.

After the sampling train has been assembled, turn on and set the filter and probe heating systems at the desired operating temperatures. Allow time for the temperatures to stabilize. If a Viton A O-ring or other leak-free connection is used in assembling the probe nozzle to the probe liner, leak-check the train at the sampling site by plugging the nozzle and pulling a 380 mm Hg (15 in. Hg) vacuum.

Note.—A lower vacuum may be used, provided that it is not exceeded during the test.

If an asbestos string is used, do not connect the probe to the train during the leak-check. Instead, leak-check the train by first plugging the inlet to the filter holder (cyclone, if applicable) and pulling a 380 mm Hg (15 in. Hg) vacuum (see Note immediately above). Then connect the probe to the train and leak-check at about 25 mm Hg (1 in. Hg) vacuum; alternatively, the probe may be leak-checked with the rest of the sampling train, in one step, at 380 mm Hg (15 in. Hg) vacuum. Leakage rates in excess of 4 percent of the average sampling rate or 0.00057 m<sup>3</sup>/min (0.02 cfm), whichever is less, are unacceptable.

The following leak-check instructions for the sampling train described in APTD-0576 and APTD-0581 may be helpful. Start the pump with bypass valve fully open and coarse adjust valve completely closed. Partially open the coarse adjust valve and slowly close the bypass valve until the desired vacuum is reached. Do not reverse direction of bypass valve; this will cause water to back up into the filter holder. If the desired vacuum is exceeded, either leak-check at this higher vacuum or end the leak check as shown below and start over.

When the leak-check is completed, first slowly remove the plug from the inlet to the probe, filter holder, or cyclone (if applicable), and immediately turn off the vacuum pump. This prevents the water in the impingers from being forced backward into the filter holder and silica gel from being entrained backward into the third impinger.

**4.1.4.2 Leak-Checks During Sample Run.** If during the sampling run, a component (e.g., filter assembly or impinger) change becomes necessary, a leak-check shall be conducted immediately before the change is made. The leak-check shall be done according to the procedure outlined in Section 4.1.4.1 above, except that it shall be done at a vacuum equal to or greater than the maximum value recorded up to that point in the test. If the leakage rate is found to be no greater than 0.00057 m<sup>3</sup>/min (0.02 cfm) or 4 percent of the average sampling rate (whichever is less), the results are acceptable, and no correction will need to be applied to the total volume of dry gas metered; if, however, a higher leakage rate is obtained, the tester shall either record the leakage rate and plan to correct the sample volume as shown in Section 6.3 of this method, or shall void the sampling run.

Immediately after component changes, leak-checks are optional; if such leak-checks are done, the procedure outlined in Section 4.1.4.1 above shall be used.

**4.1.4.3 Post-test Leak-Check.** A leak-check is mandatory at the conclusion of each sampling run. The leak-check shall be done in accordance with the procedures outlined in Section 4.1.4.1, except that it shall be conducted at a vacuum equal to or greater than the maximum value reached during the sampling run. If the leakage rate is found to be no greater than 0.00057 m<sup>3</sup>/min (0.02 cfm) or 4 percent of the average sampling rate (whichever is less), the results are acceptable, and no correction need be applied to the total volume of dry gas metered; if, however, a higher leakage rate is obtained, the tester shall either record the leakage rate and correct the sample volume as shown in Section 6.3 of this method, or shall void the sampling run.

**4.1.5 Particulate Train Operation.** During the sampling run, maintain an isokinetic sampling rate (within 10 percent of true isokinetic unless otherwise specified by the Administrator) and a temperature around the filter of 120 $\pm$ 14° C (248 $\pm$ 25° F), or such other temperature as specified by an applicable subpart of the standards or approved by the Administrator.

For each run, record the data required on a data sheet such as the one shown in Figure 5-2. Be sure to record the initial dry gas meter reading. Record the dry gas meter readings at the beginning and end of each sampling time increment, when changes in flow rates are made, before and after each leak check, and when sampling is halted.



**RULES AND REGULATIONS**

fitting, probe liner, and front half of the filter holder by washing these components with acetone and placing the wash in a glass container. Distilled water may be used instead of acetone when approved by the Administrator and shall be used when specified by the Administrator; in these cases, save a water blank and follow the Administrator's directions on analysis. Perform the acetone rinses as follows:

Carefully remove the probe nozzle and clean the inside surface by rinsing with acetone from a wash bottle and brushing with a nylon bristle brush. Brush until the acetone rinse shows no visible particles, after which make a final rinse of the inside surface with acetone.

Brush and rinse the inside parts of the Swagelok fitting with acetone in a similar way until no visible particles remain.

Rinse the probe liner with acetone by tilting and rotating the probe while squirting acetone into its upper end so that all inside surfaces will be wetted with acetone. Let the acetone drain from the lower end into the sample container. A funnel (glass or polyethylene) may be used to aid in transferring liquid wastes to the container. Follow the acetone rinse with a probe brush. Hold the probe in an inclined position, squirt acetone into the upper end as the probe brush is being pushed with a twisting action through the probe; hold a sample container underneath the lower end of the probe, and catch any acetone and particulate matter which is brushed from the probe. Run the brush through the probe three times or more until no visible particulate matter is carried out with the acetone or until none remains in the probe liner on visual inspection. With stainless steel or other metal probes, run the brush through in the above prescribed manner at least six times since metal probes have small crevices in which particulate matter can be entrapped. Rinse the brush with acetone, and quantitatively collect these washings in the sample container. After the brushing, make a final acetone rinse of the probe as described above.

It is recommended that two people be used to clean the probe to minimize sample losses. Between sampling runs, keep brushes clean and protected from contamination.

After ensuring that all joints have been wiped clean of silicone grease, clean the inside of the front half of the filter holder by rubbing the surfaces with a nylon bristle brush and rinsing with acetone. Rinse each surface three times or more if needed to remove visible particulate. Make a final rinse of the brush and filter holder. Carefully rinse out the glass cyclone, also (if applicable). After all acetone washings and particulate matter have been collected in the sample container, tighten the lid on the sample container so that acetone will not leak out when it is shipped to the laboratory. Mark the height of the fluid level to determine whether or not leakage occurred during transport. Label the container to clearly identify its contents.

**Container No. 3.** Note the color of the indicating silica gel to determine if it has been completely spent and make a notation of its condition. Transfer the silica gel from the fourth impinger to its original container and seal. A funnel may make it easier to pour the silica gel without spilling. A rubber policeman may be used as an aid in removing the silica gel from the impinger. It is not necessary to remove the small amount of dust particles that may adhere to the impinger wall and are difficult to remove. Since the gain in weight is to be used for moisture calculations, do not use any water or other liquids to transfer the silica gel. If a balance is available in the field, follow the procedure for container No. 3 in Section 4.3.

**Impinger Water.** Treat the impingers as follows: Make a notation of any color or film in the liquid catch. Measure the liquid which is in the first three impingers to within ±1 ml by using a graduated cylinder or by weighing it to within ±0.5 g by using a balance (if one is available). Record the volume or weight of liquid present. This information is required to calculate the moisture content of the effluent gas.

Discard the liquid after measuring and recording the volume or weight, unless analysis of the impinger catch is required (see Note, Section 2.1.7).

If a different type of condenser is used, measure the amount of moisture condensed either volumetrically or gravimetrically.

Whenever possible, containers should be shipped in such a way that they remain upright at all times.

**4.3 Analysis.** Record the data required on a sheet such as the one shown in Figure 5-3. Handle each sample container as follows:

**Container No. 1.** Leave the contents in the shipping container or transfer the filter and any loose particulate from the sample container to a tared glass weighing dish. Desiccate for 24 hours in a desiccator containing anhydrous calcium sulfate. Weigh to a constant weight and report the results to the nearest 0.1 mg. For purposes of this Section, 4.3, the term "constant weight" means a difference of no more than 0.3 mg or 1 percent of total weight less tare weight, whichever is greater, between two consecutive weighings, with no less than 6 hours of desiccation time between weighings.

Part \_\_\_\_\_

Date \_\_\_\_\_

Run No. \_\_\_\_\_

Filter No. \_\_\_\_\_

Amount liquid lost during transport \_\_\_\_\_

Acetone blank volume, ml \_\_\_\_\_

Acetone wash volume, ml \_\_\_\_\_

Acetone blank concentration, mg/mg (equation 5-4) \_\_\_\_\_

Acetone wash blank, mg (equation 5-5) \_\_\_\_\_

CONTAINER NUMBER	WEIGHT OF PARTICULATE COLLECTED, mg		
	FINAL WEIGHT	TARE WEIGHT	WEIGHT GAIN
1			
2			
TOTAL			
	Less acetone blank		
	Weight of particulate matter		

	VOLUME OF LIQUID WATER COLLECTED	
	IMPINGER VOLUME, ml	SILICA GEL WEIGHT, g
FINAL		
INITIAL		
LIQUID COLLECTED		
TOTAL VOLUME COLLECTED		g* ml

\* CONVERT WEIGHT OF WATER TO VOLUME BY DIVIDING TOTAL WEIGHT INCREASE BY DENSITY OF WATER (1g/ml).

$$\frac{\text{INCREASE, g}}{1 \text{ g/ml}} = \text{VOLUME WATER, ml}$$

Figure 5-3. Analytical data.

67

Alternatively, the sample may be oven dried at 105° C (220° F) for 2 to 3 hours, cooled in the desiccator, and weighed to a constant weight, unless otherwise specified by the Administrator. The tester may also opt to oven dry the sample at 105° C (220° F) for 2 to 3 hours, weigh the sample, and use this weight as a final weight.

**Container No. 5.** Note the level of liquid in the container and confirm on the analysis sheet whether or not leakage occurred during transport. If a noticeable amount of leakage has occurred, either void the sample or use methods, subject to the approval of the Administrator, to correct the final results. Measure the liquid in this container either volumetrically to ±1 ml or gravimetrically to ±0.5 g. Transfer the contents to a tared 250-ml beaker and evaporate to dryness at ambient temperature and pressure. Desiccate for 24 hours and weigh to a constant weight. Report the results to the nearest 0.1 mg.

**Container No. 5.** Weigh the spent silica gel for silica gel plus impinger) to the nearest 0.5 g using a balance. This step may be conducted in the field.

**"Acetone Blank" Container.** Measure acetone in this container either volumetrically or gravimetrically. Transfer the acetone to a tared 250-ml beaker and evaporate to dryness at ambient temperature and pressure. Desiccate for 24 hours and weigh to a constant weight. Report the results to the nearest 0.1 mg.

**NOTE.**—At the option of the tester, the contents of Container No. 2 as well as the acetone blank container may be evaporated at temperatures higher than ambient. If evaporation is done at an elevated temperature, the temperature must be below the boiling point of the solvent; also, to prevent "bumping," the evaporation process must be closely supervised, and the contents of the beaker must be swirled occasionally to maintain an even temperature. Use extreme care, as acetone is highly flammable and has a low flash point.

**5. Calibration**

Maintain a laboratory log of all calibrations.

**5.1 Probe Nozzle.** Probe nozzles shall be calibrated before their initial use in the field. Using a micrometer, measure the inside diameter of the nozzle to the nearest

0.025 mm (0.001 in.). Make three separate measurements using different diameters each time, and obtain the average of the measurements. The difference between the high and low numbers shall not exceed 0.1 mm (0.004 in.). When nozzles become nicked, dented, or corroded, they shall be reshaped, sharpened, and recalibrated before use. Each nozzle shall be permanently and uniquely identified.

**5.2 Pitot Tube.** The Type 8 pitot tube assembly shall be calibrated according to the procedure outlined in Section 4 of Method 2.

**5.3 Metering System.** Before its initial use in the field, the metering system shall be calibrated according to the procedure outlined in APTD-0578. Instead of physically adjusting the dry gas meter dial readings to correspond to the wet test meter readings, calibration factors may be used to mathematically correct the gas meter dial readings to the proper values. Before calibrating the metering system, it is suggested that a leak-check be conducted. For metering systems having diaphragm pumps, the normal leak-check procedure will not detect leakages within the pump. For these cases the following leak-check procedure is suggested: make a 10-minute calibration run at 0.00057 m<sup>3</sup>/min (0.02 cfm); at the end of the run, take the difference of the measured wet test meter and dry gas meter volumes; divide the wet test meter to get the leak rate. The leak rate should not exceed 0.00057 m<sup>3</sup>/min (0.02 cfm).

After each field use, the calibration of the metering system shall be checked by performing three calibration runs at a single, intermediate orifice setting (based on the previous field test), with the vacuum set at the maximum value reached during the test series. To adjust the vacuum, insert a valve between the wet test meter and the inlet of the metering system. Calculate the average value of the calibration factor. If the calibration has changed by more than 5 percent, recalibrate the meter over the full range of orifice settings, as outlined in APTD-0578.

Alternative procedures, e.g., using the orifice meter coefficients, may be used, subject to the approval of the Administrator.

**NOTE.**—If the dry gas meter coefficient values obtained before and after a test series differ by more than 5 percent, the test series shall either be voided, or calculations for the test series shall be performed using whichever meter coefficient value (i.e., before or after) gives the lower value of total sample volume.

**5.4 Probe Heater Calibration.** The probe heating system shall be calibrated before its initial use in the field according to the procedure outlined in APTD-0578. Probes constructed according to APTD-0581 need not be calibrated if the calibration curves in APTD-0578 are used.

**5.5 Temperature Gauges.** Use the procedure in Section 4.3 of Method 2 to calibrate in-stack temperature gauges. Dial thermometers, such as are used for the dry gas meter and condenser outlet, shall be calibrated against mercury-in-glass thermometers.

**5.6 Leak Check of Metering System Shown in Figure 5-1.** That portion of the sampling train from the pump to the orifice meter should be leak checked prior to initial use and after each shipment. Leakage after the pump will result in less volume being recorded than is actually sampled. The following procedure is suggested (see Figure 5-4): Close the main valve on the meter box. Insert a one-hole rubber stopper with rubber tubing attached into the orifice exhaust pipe. Disconnect and vent the low side of the orifice manometer. Close off the (6 to 7 in.) water column by blowing into the rubber tubing. Pinch off the tubing and observe the manometer for one minute. A loss of pressure on the manometer indicates a leak in the meter box; leaks, if present, must be corrected.

**5.7 Barometer.** Calibrate against a mercury barometer.

**6. Calculations**

Carry out calculations, retaining at least one extra decimal figure beyond that of the acquired data. Round off figures after the final calculation. Other forms of the equations may be used as long as they give equivalent results.

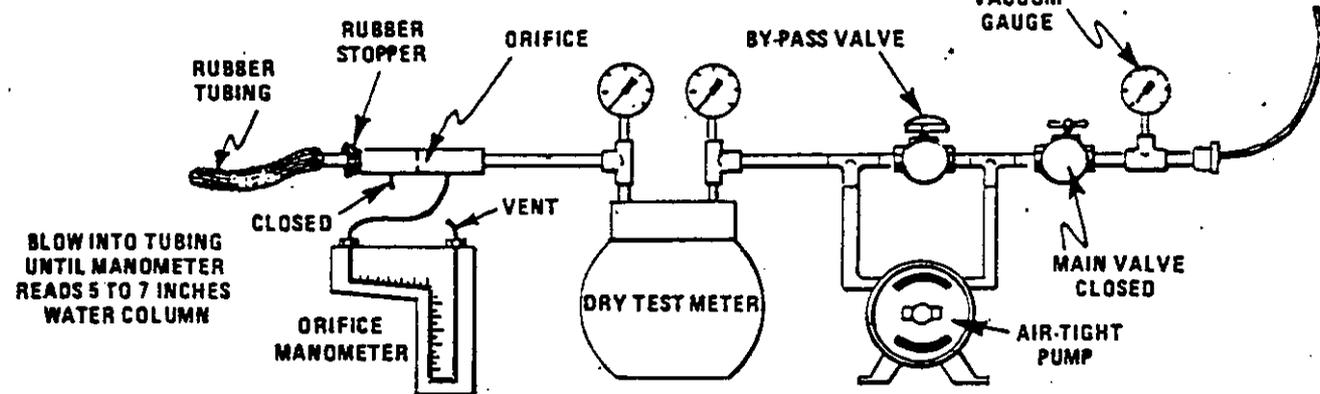


Figure 5-4. Leak check of meter box.

**6.1 Nomenclature**

- A<sub>1</sub> = Cross-sectional area of nozzle, m<sup>2</sup> (ft<sup>2</sup>).
- B<sub>w</sub> = Water vapor in the gas stream, proportion by volume.
- C<sub>1</sub> = Acetone blank reading concentrations, mg/g.
- C<sub>2</sub> = Concentration of particulate matter in stack gas, dry basis, corrected to standard conditions, g/dscfm (g/dscf).
- I = Percent of isokinetic sampling.
- L<sub>1</sub> = Maximum acceptable leakage rate for either a pre-test leak check or for a leak check following a component change; equal to 0.00057 m<sup>3</sup>/min (0.02 cfm) or 4 percent of the average sampling rate, whichever is less.
- L<sub>2</sub> = Individual leakage rate observed during the leak check conducted prior to the "n<sup>th</sup>" component change (i=1, 2, 3, . . . , n), m<sup>3</sup>/min (cfm).
- L<sub>3</sub> = Leakage rate observed during the post-test leak check, m<sup>3</sup>/min (cfm).
- m<sub>a</sub> = Total amount of particulate matter collected, mg.
- M<sub>w</sub> = Molecular weight of water, 18.0 g/g-mole (18.0 lb/lb-mole).
- m<sub>s</sub> = Mass of residue of acetone after evaporation, mg.
- P<sub>bar</sub> = Barometric pressure at the sampling site, mm Hg (in. Hg).
- P<sub>std</sub> = Absolute stack gas pressure, mm Hg (in. Hg).
- P<sub>std</sub> = Standard absolute pressure, 760 mm Hg (29.92 in. Hg).

- R = Ideal gas constant, 0.08206 mm Hg-m<sup>3</sup>/°K-g-mole (21.85 in. Hg-ft<sup>3</sup>/°R-lb-mole).
- T<sub>a</sub> = Absolute average dry gas meter temperature (see Figure 5-2), °K (°F).
- T<sub>s</sub> = Absolute average stack gas temperature (see Figure 5-2), °K (°F).
- T<sub>std</sub> = Standard absolute temperature, 293° K (528° F).
- V<sub>1</sub> = Volume of acetone blank, ml.
- V<sub>2</sub> = Volume of acetone used in wash, ml.
- V<sub>1+2</sub> = Total volume of liquid collected in impingers and silica gel (see Figure 5-3), ml.
- V<sub>3</sub> = Volume of gas sample as measured by dry gas meter, dscm (dscf).
- V<sub>4(i+1)</sub> = Volume of gas sample measured by the dry gas meter, corrected to standard conditions, dscm (dscf).
- V<sub>4(i+2)</sub> = Volume of water vapor in the gas sample, corrected to standard conditions, scm (scf).
- V<sub>5</sub> = Stack gas velocity, calculated by Method 1, Equation 2-9, using data obtained from Method 5, m/sec (ft/sec).
- W<sub>1</sub> = Weight of residue in acetone wash, mg.
- Y = Dry gas meter calibration factor.
- ΔH = Average pressure differential across the orifice meter (see Figure 5-2), mm H<sub>2</sub>O (in. H<sub>2</sub>O).
- ρ<sub>a</sub> = Density of acetone, mg/ml (see label on bottle).
- ρ<sub>w</sub> = Density of water, 0.9982 g/ml (0.02201 lb/ml).
- t = Total sampling time, min.

- θ<sub>1</sub> = Sampling time interval, from the beginning of a run until the first component change, min.
- θ<sub>2</sub> = Sampling time interval, between two successive component changes, beginning with the interval between the first and second changes, min.
- θ<sub>3</sub> = Sampling time interval, from the final (n<sup>th</sup>) component change until the end of the sampling run, min.

- 13.6 = Specific gravity of mercury, 80-sec/mm.
- 100 = Conversion to percent.
- 6.3 Average dry gas meter temperature and average orifice pressure drop. See data sheet (Figure 5-2).
- 6.3 Dry Gas Volume. Correct the sample volume measured by the dry gas meter to standard conditions (20° C, 760 mm Hg or 68° F, 29.92 in. Hg) by using Equation 5-1.

$$V_{4(i+2)} = V_4 Y \left( \frac{T_{std}}{T_a} \right) \left[ \frac{P_{bar} + \Delta H}{P_{std}} \right]$$

$$= K_1 V_4 Y \frac{P_{bar} + (\Delta H/13.6)}{T_a}$$

Equation 5-1

where:

$$m_1 = 0.3856 \text{ } ^\circ\text{K/mm Hg for metric units} \\ = 17.84 \text{ } ^\circ\text{E/in. Hg for English units}$$

NOTE.—Equation 5-1 can be used as written unless the leakage rate observed during any of the mandatory leak checks (i.e., the post-test leak check or leak checks conducted prior to component changes) exceeds  $L_{10}$ . If  $L_{10}$  or  $L_1$  exceeds  $L_{10}$ , Equation 5-1 must be modified as follows:

(a) Case I. No component changes made during sampling run. In this case, replace  $V_m$  in Equation 5-1 with the expression:

$$V_m = (L_p - L_{10})\theta$$

(b) Case II. One or more component changes made during the sampling run. In this case, replace  $V_m$  in Equation 5-1 by the expression:

$$\left[ V_m - (L_1 - L_{10})\theta_1 \right. \\ \left. - \sum_{i=2}^n (L_i - L_{10})\theta_i - (L_p - L_{10})\theta_p \right]$$

and substitute only for those leakage rates ( $L_i$  or  $L_p$ ) which exceed  $L_{10}$ .

6.4 Volume of water vapor.

Equation 5-2

$$V_{w(std)} = V_{10} \left( \frac{p_w}{M_w} \right) \left( \frac{RT_{std}}{P_{std}} \right) = K_2 V_{10}$$

where:

$$K_2 = 0.001233 \text{ m}^3/\text{ml for metric units} \\ = 0.04707 \text{ ft}^3/\text{ml for English units}$$

6.5 Moisture Content.

$$B_{w,s} = \frac{V_{w(std)}}{V_m(std) + V_{w(std)}}$$

Equation 5-3

$$I = \frac{100 T_s [K_1 V_{10} + (V_m/T_m) (P_{bar} + \Delta H/13.6)]}{60 \theta v_s P_s A_s}$$

Equation 5-7

where:

$$K_1 = 0.003454 \text{ mm Hg} \cdot \text{m}^3/\text{ml} \cdot ^\circ\text{K for metric units} \\ = 0.002669 \text{ in. Hg} \cdot (\text{ft}^3/\text{ml}) \cdot ^\circ\text{R for English units}$$

6.11.2 Calculation From Intermediate Values.

$$I = \frac{T_s V_m(std) P_{std} 100}{T_{std} \theta v_s \theta A_s P_s 60 (1 - B_{w,s})} \\ = K_3 \frac{T_s V_m(std)}{P_s V_s A_s \theta (1 - B_{w,s})}$$

Equation 5-8

where:

$$K_3 = 4.320 \text{ for metric units} \\ = 0.09450 \text{ for English units}$$

6.12 Acceptable Results. If 90 percent  $\leq I \leq 110$  percent, the results are acceptable. If the results are low in comparison to the standard and  $I$  is beyond the acceptable range, or, if  $I$  is less than 90 percent, the Administrator may opt to accept the results. Use Citation 4 to make judgments. Otherwise, reject the results and repeat the test.

#### 7. Bibliography

1. Addendum to Specifications for Incinerator Testing at Federal Facilities. PHS, NCAPC, Dec. 6, 1967.
2. Martin, Robert M. Construction Details of Isokinetic Source-Sampling Equipment. Environmental Protection Agency, Research Triangle Park, N.C. APTD-0681, April, 1971.
3. Bora, Jerome J. Maintenance, Calibration, and Operation of Isokinetic Source Sampling Equipment. Environmental Protection Agency, Research Triangle Park, N.C. APTD-0576, March, 1972.
4. Smith, W. S., R. T. Shigehara, and W. F. Todd. A Method of Interpreting Stack Sampling Data. Paper Presented at the 63d Annual Meeting of the Air Pollution Control Association, St. Louis, Mo. June 14-19, 1970.
5. Smith, W. S., et al. Stack Gas Sampling Improved and Simplified With New Equipment. APCA Paper No. 67-119, 1967.
6. Specifications for Incinerator Testing at Federal Facilities. PHS, NCAPC, 1967.
7. Shigehara, R. T. Adjustments in the EPA Nomograph for Different Pitot Tube Coefficients and Dry Molecular Weights. Stack Sampling News 24-25, October, 1974.

NOTE.—In saturated or water droplet-laden gas streams, two calculations of the moisture content of the stack gas shall be made, one from the impinger analysis (Equation 5-3), and a second from the assumption of saturated conditions. The lower of the two values of  $B_{w,s}$  shall be considered correct. The procedure for determining the moisture content based upon assumption of saturated conditions is given in the Note of Section 1.2 of Method 4. For the purposes of this method, the average stack gas temperature from Figure 5-2 may be used to make this determination, provided that the accuracy of the in-stack temperature sensor is  $\pm 1^\circ\text{C}$  ( $2^\circ\text{F}$ ).

6.6 Acetone Blank Concentration.

$$C_a = \frac{m_a}{V_a \rho_a}$$

Equation 5-4

6.7 Acetone Wash Blank.

$$W_a = C_a V_{aw} \rho_a$$

Equation 5-5

6.8 Total Particulate Weight. Determine the total particulate catch from the sum of the weights obtained from containers 1 and 2 less the acetone blank (see Figure 5-3). NOTE.—Refer to Section 4.1.5 to assist in calculation of results involving two or more filter assemblies or two or more sampling trains.

6.9 Particulate Concentration.

$$c_p = (0.001 \text{ g/mg}) (m_p/V_m(std))$$

Equation 5-6

6.10 Conversion Factors:

From	To	Multiply by
scf	m <sup>3</sup>	0.70832
g/ft <sup>3</sup>	gr/ft <sup>3</sup>	15.43
g/ft <sup>3</sup>	lb/ft <sup>3</sup>	2.205 × 10 <sup>-3</sup>
g/ft <sup>3</sup>	g/m <sup>3</sup>	35.31

6.11 Isokinetic Variation:

6.11.1 Calculation From Raw Data.

8. Voliani, R. F. A Survey of Commercially Available Instrumentation For the Measurement of Low-Range Gas Velocities. U.S. Environmental Protection Agency, Emission Measurement Branch, Research Triangle Park, N.C. November, 1976 (unpublished paper).

9. Annual Book of ASTM Standards, Part 23, Gaseous Fuels; Coal and Coke; Atmospheric Analysis. American Society for Testing and Materials, Philadelphia, Pa. 1974, pp. 617-622.

#### METHOD 6—DETERMINATION OF SULFUR DIOXIDE EMISSIONS FROM STATIONARY SOURCES

##### 1. Principle and Applicability

1.1 Principle. A gas sample is extracted from the sampling point in the stack. The sulfuric acid mist (including sulfur trioxide) and the sulfur dioxide are separated. The sulfur dioxide fraction is measured by the barium-thorium titration method.

1.2 Applicability. This method is applicable for the determination of sulfur dioxide emissions from stationary sources. The minimum detectable limit of the method has been determined to be 3.4 milligrams (mg) of SO<sub>2</sub>/m<sup>3</sup> (2.12 × 10<sup>-4</sup> lb/ft<sup>3</sup>). Although no upper limit has been established, tests have shown that concentrations as high as 50,000 mg/m<sup>3</sup> of SO<sub>2</sub> can be collected efficiently in two midsize impingers, each containing 15 milliliters of 3 percent hydrogen peroxide, at a rate of 1.0 lpm for 20 minutes. Based on theoretical calculations, the upper concentration limit in a 20-liter sample is about 93,300 mg/m<sup>3</sup>.

Possible interferences are free ammonia, water-soluble cations, and fluorides. The cations and fluorides are removed by glass wool filters and an isopropanol bubbler, and hence do not affect the SO<sub>2</sub> analysis. When samples are being taken from a gas stream with high concentrations of very fine metallic fumes (such as in inlets to control devices), a high-efficiency glass fiber filter must be used in place of the glass wool plug (i.e., the one in the probe) to remove the cation interferences.

Free ammonia interferes by reacting with SO<sub>2</sub> to form particulate sulfite and by reacting with the indicator. If free ammonia is present (this can be determined by knowledge of the process and noticing white particulate matter in the probe and isopropanol bubbler), alternative methods, subject to the approval of the Administrator, U.S. Environmental Protection Agency, are required.

##### 2. Apparatus

STAKSAMPLER CALIBRATION SHEET

ENVIRONMENTAL TESTING, INC.	Valves OK
Date 1/5/79	Remarks: Piox # 51401
Pump OK	Ambient 20.5°C
Pump Oil OK	
Clean Quick Connects OK	
Manometers OK	
Dry Test Water OK	
Thermometers OK	
Lights OK	
Electrical Check--Amphenol OK	
Variac OK	
Vacuum Gauge OK	
Leak Check at 27" Hg.--Leakage < 0.001	

Calibration--Orifice and Meter


Date 1/5/79 Box No. S1401 P<sub>b</sub> 30.12

Man. Orifice	CF <sub>w</sub>	CF <sub>d</sub>	T <sub>w</sub>	IT <sub>d</sub>	OT <sub>d</sub>	T <sub>d</sub> avg.	Time t
0.5	5	5.21	67	90	72	81	12.49
1.0	5	5.29	67	105	78	92	9.13
2.0	10	10.56	67	116	86	101	13.16
4.0	10	10.56	67	125	93	109	9.51
6.0	10	10.45	68	130	98	114	7.70
8.0	10	10.23	69	133	102	118	6.58

Calculate Y & ΔH<sub>0</sub> at man. 2.0

$$CF_w P_b (T_d \text{ avg.} + 460)$$

$$CF_d (P_b + 0.117) (T_w + 460)$$

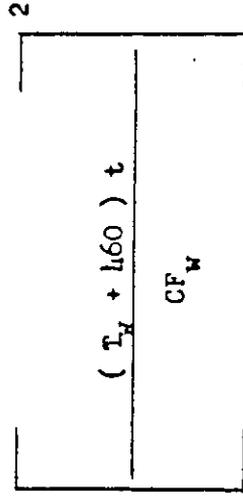

$$\Delta H_0 = \frac{0.0634}{P_b (OT_d + 460)}$$

Tolerances

$$Y = 0.99 - \frac{1.00}{1.00} - 1.01$$

$$H_0 = 1.6 - \frac{1.84}{1.84} - 2.1$$

CALIBRATION CALCULATIONS PETER AND PUMP

Date 1/5/79

Box No. 51901

		Man.	$\Delta H_g$		Man.	T
.0317 (Man. orifice)	$(T_w + 460) t$			$CF_w P_b (T_d \text{ ave.} + 460)$		
$P_b (OT_d + 460)$	$CF_w$			$CF_d \left( P_b + \frac{\text{Man. orifice}}{13.6} \right) (T_w + 460)$		
0.01585	$\frac{(67 + 460) 12.49}{5}$	.5	1.71	$5 \times 30.12 \left( \frac{81}{31} + 460 \right)$	.5	0.98
$2.12 (72 + 460)$	$\frac{(67 + 460) 9.13}{5}$	1.0	1.81	$5.21 (30.12 + 0.0368) (67 + 460)$		
0.0317	$\frac{(67 + 460) 13.16}{78}$	2.0	1.85	$10 \times 30.12 \left( \frac{101}{101} + 460 \right)$	2.0	1.00
$2.12 (78 + 460)$	$\frac{(67 + 460) 9.51}{10}$	4.0	1.91	$10.56 (30.12 + 0.294) (67 + 460)$	4.0	1.01
0.1268	$\frac{(68 + 460) 7.70}{10}$	6.0	1.87	$10 \times 30.12 \left( \frac{114}{114} + 460 \right)$	6.0	1.03
$0.12 (93 + 460)$	$\frac{(69 + 460) 6.58}{10}$	8.0	1.82	$10.45 (30.12 + 0.431) (68 + 460)$	8.0	1.05
0.2536	$\frac{(69 + 460) 6.58}{10}$			$10 \times 30.12 \left( \frac{118}{118} + 460 \right)$		
$2.12 (102 + 460)$				$10.23 (30.12 + 0.588) (69 + 460)$		